

1 Intercomparison of four different cascade impactors for 2 fine and ultrafine particle sampling in two European 3 locations

4

5 A. S. Fonseca^{1,2,*}, N. Talbot^{3,4}, J. Schwarz³, J. Ondráček³, V. Ždímal³, J.
6 Kozáková^{3,4}, M. Viana¹, A. Karanasiou¹, X. Querol¹, A. Alastuey¹, T. V. Vu⁵, J. M.
7 Delgado-Saborit⁵, R. M. Harrison^{5, †}

8 ¹ Institute of Environmental Assessment and Water Research (IDÆA-CSIC), Barcelona,
9 08034, Spain

10 ² Universidad de Barcelona, Facultad de Química, Barcelona, 08028, Spain

11 ³ Institute of Chemical Process Fundamentals of the ASCR, v.v.i. (ICPF), Prague, 165 02,
12 Czech Republic

13 ⁴Charles University in Prague, Faculty of Science, Institute for Environmental Studies,
14 Prague, 128 43, Czech Republic

15 ⁵University of Birmingham, Division of Environmental Health & Risk Management,
16 Birmingham, B15 2TT,UK

17 [†]Also at: Department of Environmental Sciences / Center of Excellence in Environmental
18 Studies, King Abdulaziz University, PO Box 80203, Jeddah, 21589, Saudi Arabia

19 *Correspondence to: A. S. Fonseca (ana.godinho@idaea.csic.es)

20

21 **Abstract**

22 Due to the need to better characterise the ultrafine particles fraction and related personal
23 exposure, several impactors have been developed to enable the collection of ultrafine particles
24 (<100 nm). However, to the authors' knowledge there have been no field campaigns to-date
25 intercomparing impactor collection of ultrafine particles. The purpose of this study was two-
26 fold: 1) to assess the performance of a number of conventional and nano-range cascade
27 impactors with regard to the particle mass size distribution under different environmental
28 conditions and aerosol loads and types, and 2) to characterise aerosol size distributions
29 including ultrafine particles using impactors in 2 European locations. The impactors used
30 were: (i) Berner low-pressure impactor (BLPI; 26 nm - 13.5 µm), (ii) nano-Berner low-

1 pressure impactor (nano-BLPI; 11 nm - 1.95 μm) and (iii) Nano-microorifice uniform deposit
2 impactor (nano-Moudi; 10 nm-18 μm), and (iv) Personal cascade impactor Sioutas (PCIS; <
3 250 nm - 10 μm). Only the BLPI substrates were coated with a thin layer of vacuum grease,
4 therefore particle bounce that may occur during dry collection should only be considered for
5 the other impactors.

6 Taking the BLPI as an internal reference, the best agreement regarding mass size distributions
7 was obtained with the nano-BLPI, independently of the aerosol load and aerosol chemical
8 composition. The nano-Moudi showed a good agreement for particle sizes >320 nm, whereas
9 for particle diameters <320 nm this instrument recorded larger mass concentrations in outdoor
10 air than the internal reference. This difference could be due to particle bounce, to the
11 dissociation of semi volatiles in the coarser stages and/or to particle shrinkage during
12 transport through the impactor due to higher temperature inside this impactor. Further
13 research is needed to understand this behaviour.

14 With regard to the PCIS, their size-resolved mass concentrations were comparable with other
15 impactors ~~for PM_{10} , PM_2 and PM_{10}~~ , but the cut-off at 250 nm did not seem to be consistent
16 with that of the internal reference.

17 **Keywords:** Mass size distribution; Chemical characterization; Ultra-fine particles; Cascade
18 Impactors; Nanoparticles; Ultrafine particles

19

20 **1 Introduction**

21 Used in numerous areas of air quality research, cascade impactors are established, relatively
22 simple, and robust instruments. They collect airborne aerosols and segregate them into a
23 number of aerodynamic sizes for subsequent determination of mass size distribution, chemical
24 and/or physical properties (Hitzenberger *et al.*, 2004; Seinfeld and Pandis, 2006). The
25 mechanical principle behind size impaction employs the known quantities of Stokes number
26 and slip correction factors to derive particle inertia, therefore ascribing a stopping distance in
27 accordance to particle size (Hinds, 1999). Particulates are collected onto substrates, frequently
28 made of quartz, polytetrafluoroethylene (PTFE; best known as Teflon), polyethylene
29 terephthalate (commonly abbreviated PET, otherwise known as Mylar), polycarbonate or
30 aluminium (Howell *et al.*, 1998; Schaap *et al.*, 2004; Tursic *et al.*, 2008). The choice of
31 substrate is dependent on the type of impactor, sampling conditions and analytical techniques

1 intended to be carried out (Fujitani *et al.*, 2006). A variety of cascade impactor designs have
2 appeared since May (1945) first reported on an initial design to sample coarse aerosols (>2.5
3 μm). Since then, sampling size fractions for traditionally designed commercially available
4 cascade impactors allowed for particle collection from coarse to fine fractions ($<2.5 \mu\text{m}$), for
5 example $10 \mu\text{m} - 0.034 \mu\text{m}$ for the Berner low-pressure impactor (BLPI) (Hering *et al.*, 1978;
6 Berner and Luerzer, 1980; Hillamo and Kauppinen, 1991) and size cuts as small as $0.056 \mu\text{m}$
7 for the micro-orifice uniform deposit impactor (Moudi) (Marple *et al.*, 1991).

8 However, epidemiological studies have evidenced the need to focus on ultrafine particles
9 (UFP; $D_p < 100 \text{ nm}$), due to their possibly larger impacts on health when compared to coarser
10 particles (Oberdörster, 2000; Oberdorster *et al.*, 2005). Recently, due to the growing need to
11 better characterise the UFP fraction, the second generation of Moudi impactors (Model 122
12 and Model 125 Nano-Moudi-II™, MSP Corp., Shoreview, MN, USA), both available in the
13 rotating version (122-R and 125-R) and in the non-rotating version (122-NR and 125-NR) and
14 nano-BLPI (not commercially available) were introduced, both adaptations of the original
15 Moudi (Marple *et al.*, 1991) and BLPI impactors (Hering *et al.*, 1978; Berner and Luerzer,
16 1980; Hillamo and Kauppinen, 1991), modified to enable the collection of UFP down to 11
17 nm. Also, the need to better understand and characterise personal exposure led to the
18 development of portable, light-weight impactors such as the personal cascade impactor
19 sampler (PCIS; Misra *et al.*, 2002).

20 Due to the physical principle of particle collection associated with all impactors sampling
21 artefacts can occur, including particle bounce, particle blow off, and particle wall loss (Wall *et*
22 *al.*, 1988; Schwarz *et al.*, 2012). These artefacts vary according to the impactor type (Hillamo
23 and Kauppinen, 1991; Howell *et al.*, 1998; Štefancová *et al.*, 2011) loads, composition of the
24 aerosol sampled (Huang *et al.*, 2004; Sardar *et al.*, 2005; Fujitani *et al.*, 2006; Crilley *et al.*,
25 2013), and the type of substrate used (Fujitani *et al.*, 2006; Nie *et al.*, 2010). Also, because
26 long sampling time is required for having enough mass of the finest UFP for chemical
27 analysis may produce sampling artefacts of volatilization or absorption.

28 As well as those previously described, the sampling and accurate sizing of UFP/nanoparticles
29 also present challenges. There is a need to produce a fast flowing jet of air onto an impactor
30 plate, creating the inertia allowing for collection of the smallest size fractions producing a
31 high pressure differential at the lowest cut sizes. This pressure drop changes the vapour
32 pressure in the bulk which can then enhance volatilisation (Hering and Cass, 1999). Attempts

1 to address this issue were successfully carried out by decreasing the pressure drop over a
2 reduced number of stages (Marple *et al.*, 1991; Štefancová *et al.*, 2011). Moreover, the low
3 mass of UFP requires a greater collection concentration which then increases the possibility
4 of mass overloading on the larger fractions. The commercially available Nano-Moudi-
5 II™ seeks to reduce jet velocity, pressure drop, particle bounce, re-entrainment and
6 evaporative loss by incorporating micro-orifice nozzles (up to 2000 as small as 50 µm in
7 diameter in the 10 L/min Model 125 and up to 6 000 of 50 µm diameter in the 30 L min⁻¹
8 Model 122). The rotating Nano-Moudi-II™ versions (Model 122-R and 125-R) have internal
9 embedded stepper motors for the rotation of the sampling stages, thereby spreading the
10 sample over the filter to reduce build-up (Marple *et al.*, 2014). However, as will be described
11 below, this spreading of the sample may lead to new uncertainties and complications.

12 Cascade impactors have been deployed in a diverse array of measurement campaigns utilising
13 their versatility, characterising size-fractionated chemical composition of urban aerosols
14 (Sardar *et al.*, 2005; Schwarz *et al.*, 2012), particle volatility (Hering and Cass, 1999; Huang
15 *et al.*, 2004), vapour-particle phase partitioning (Delgado-Saborit *et al.*, 2014), influence of
16 relative humidity (Štefancová *et al.*, 2010), indoor - outdoor relationship (Smolík *et al.*,
17 2008), archive contamination (Mašková *et al.*, 2015), metals in particles collected near a busy
18 road (Lin *et al.*, 2005; Karanasiou *et al.*, 2007; Ondráček *et al.*, 2011), size-segregated
19 emission particles in a coal-fired power station (Tursic *et al.*, 2008), whilst extensive
20 theoretical investigations and experimental characterization of cascade impactors tended to
21 focus on the performance of one type of cascade impactor (Biswas and Flagan, 1984; Wang
22 and John, 1988; Štefancová *et al.*, 2011; Jiménez and Ballester, 2011; Marple *et al.*, 2014).
23 Howell *et al.* (1998) carried out an intercomparison of ‘traditional’ BLPI and Moudi
24 impactors during a field campaign. Field campaigns usually provide a greater variation of
25 conditions than controlled laboratory based conditions, offering a more robust analysis of
26 comparable instrumentation. Another notable intercomparison study was conducted by
27 Pennanen *et al.* (2007) who tested a modified 4-stage Harvard high-volume cascade impactor
28 against a reference 10-stage BLPI in 6 different European locations over different seasons.
29 The authors note the implicit effects on individual impactors of meteorology and aerosol
30 composition. Other studies have run two or more impactors in tandem measuring
31 simultaneously indoors and outdoors (Smolík *et al.*, 2008; Mašková *et al.*, 2015), to cover
32 extended particle size distributions (Geller *et al.*, 2002), or characterise artefacts caused by

1 particle volatility (Huang *et al.*, 2004; Schaap *et al.*, 2004) or changes in size distribution due
2 to different relative humidity (Štefancová *et al.*, 2010).

3 To the authors' knowledge there has been no field campaign to-date intercomparing impactor
4 collection efficiency of UFP. As a result, this paper seeks to address this by assessing the
5 performance of a number of conventional and nano-range impactors, namely Berner low-
6 pressure impactor (BLPI, 25/0.018/2, Hauke, Austria), nano-Berner low-pressure impactor
7 (nano-BLPI, 10/0,01, Hauke, Austria), nano-microorifice uniform deposit impactor (Nano-
8 Moudi-II™, MSP Corp., Shoreview, MN, USA Model 125R; U.S. Patent # 6,431,014B1) and
9 Personal cascade impactor Sioutas (Sioutas™ PCIS, SKC Inc.; Misra *et al.*, 2002), by means
10 of two intercomparison exercises, one in Prague, during winter 2015, and other in Barcelona
11 during summer 2015. The aim of the campaigns was to test the instruments' performance
12 under different environmental conditions and aerosol loads and types. Our work reports on the
13 impactor performances not only with regard to different particle size distributions but also
14 aerosol composition and meteorology.

15 **2 Methodology**

16 **2.1 Sampling sites and sampling set-up**

17 *2.1.1 Prague*

18 The field intercomparison initially took place in outdoor air (6th-23rd February 2015) and it
19 was subsequently moved indoors (23rd February 2015 - 2nd March 2015) in Prague, Suchdol at
20 the Institute of Chemical Process Fundamentals (ICPF), Academy of Sciences of the Czech
21 Republic (ASCR) compound (50°7'36.47"N, 14°23'5.51"E, 277 m.a.s.l). Suchdol is a
22 residential area in north-western Prague, about 6 km from the city centre. It is recognized as a
23 suburban background site with residential houses and a university campus interspersed
24 between plenty of green spaces. The traffic flow is moderate along one major 2-lane road
25 (average traffic of 10000-15000 vehicles day⁻¹) with regular bus services. Due to its location
26 on a plateau above the river Vltava there are not many contributory roads alongside (Figure
27 | [S1 in the supplementary information](#)). Detailed information of the area where the impactors
28 were located were previously provided by Smolík *et al.* (2008) and Hussein *et al.* (2006).

29 Outdoor sampling consisted of 3 weekend sampling periods (6 - 9th, 13 - 16th and 20th - 23rd
30 | February 2015), and 2 week-day samplings, (10 - 12th and 17 - 20st [February 2015](#)).

1 In addition, indoor samples were also collected during 2 week-day samplings (23rd - 25th and
2 25th - 27th February 2015) and a final 3-day weekend sampling period (27th February 2015 -
3 2nd March 2015). This resulted in a total of 5 valid outdoor samples (three weekend and two
4 week-day) and two valid indoor samples (one weekend and one week-day). For both outdoor
5 and indoor sampling, the weekend runs started on the preceding Friday between 11:00h-
6 13:00h local time and finished at 9:00h local time on the following Monday. The week-day
7 samplings started between 11h00-14h00 and terminated at 9h00. The sample duration in
8 Prague was defined based on the experience from previous research (Smolík *et al.*, 2008;
9 Štefancová *et al.*, 2011). Based on ambient PM concentrations it was considered that samples
10 should be collected over no more than 72 hours, to avoid substrate overload.

11 2.1.2 Barcelona

12 The Barcelona intercomparison was conducted exclusively outdoors at an air quality
13 monitoring station at IDAEA-CSIC located in an urban background site in the southwest of
14 Barcelona (41°23'14" N, 02°06'56"E, 78 m.a.s.l) from 18th May to 3rd July 2015 (Figure S2
15 [in the supplementary information](#)). The sampling site, described in detail by Reche *et al.*
16 (2015), is influenced by vehicular emissions from one of the city's main traffic avenues
17 (Diagonal avenue), located at approximately 200 m from the site and with a mean traffic
18 density of 90 000 vehicles/day $L^{-1}min^{-1}$ (Amato *et al.*, 2015). Even though the site is officially
19 classified as urban background, it is located in a city with very high road traffic and
20 influenced by the emissions of one of the largest arterial roads of the city.

21 [Outdoor sampling in Barcelona consisted of 4-day \(during week-days\) samples, each of them](#)
22 [accounting for 96h \(4 consecutive days\). A total of 4 samples \(4-days each\) was collected.](#)

23 The runs started every Monday between 10:00h-12:00h local time and finished on Fridays
24 around 14:00h-16:00h local time. The sample duration in Barcelona was set longer than in
25 Prague since the averages of particle mass collected during a sampling less than 4 days would
26 not be sufficient for further chemical analysis. Indoor intercomparisons were not carried out
27 due to the absence of an appropriate location for indoor air sampling.

28 2.2 Instrument set-up and experimental specifications

29 In the present study, the mass size distribution of the aerosol was measured by different types
30 of cascade impactors:

- 1 ■ A Berner low-pressure impactor (BLPI, 25/0.018/2, Hauke, Austria; (Berner et al., 1979;
2 Preining and Berner, 1979) which collects particles onto PET foils (Mylar 13 μm thick)
3 (flow rate 24.8 L min^{-1}). The impactors separated particle mass into 10 size fractions. The
4 cut diameters of the stages were 0.026, 0.056, 0.1, 0.16, 0.25, 0.43, 0.86, 1.73, 3.425, and
5 6.61 μm (Štefancová *et al.*, 2011). The impactors were equipped with inlets with the cut-
6 point calculated as 14 μm .
- 7 ■ A modified BLPI (denominated as nano-BLPI, 10/0.01, Hauke, Austria) collecting
8 particles on PET foils (Mylar 13 μm thick) (flow rate 17.2 L min^{-1}) from 0.01 μm to 1.95
9 μm in 8 size stages. The aerodynamic cut diameters of stages 1 to 8 were 0.011, 0.024,
10 0.039, 0.062, 0.095, 0.24, 0.49, 1.0 μm , and the inlet cut-point was calculated as 1.95 μm .
11 Given that the nano-BLPI is a custom made instrument, the design parameters of each of
12 its impaction stages are shown in Table S1 in the [supplementary supporting](#) information.
- 13 ■ A nano-microorifice uniform deposit area impactor (Nano-Moudi-II™, MSP Corp.,
14 Shoreview, MN, USA Model 125R; U.S. Patent # 6,431,014B1) equipped with PTFE
15 filters (with diameters of 47 mm, [0.5 \$\mu\text{m}\$ pore and 0.14 mm thick](#)) was used to collect
16 size-resolved aerosol samples.
- 17 ■ This impactor effectively separated the particulate matter into 13 stages with nominal cut
18 diameters of 0.010, 0.018, 0.03, 0.06, 0.10, 0.18, 0.32, 0.56, 1.0, 1.8, 3.2, 5.6, 10 μm and
19 the inlet cut-point as 18 μm when operated at an inlet flow rate of 10 L min^{-1} .
- 20 ■ Three personal cascade impactor samplers (Sioutas™ PCIS, SKC Inc; Misra *et al.*, 2002)
21 operating with a flow rate of 9 L min^{-1} at a pressure drop of 11 inches of H_2O (2.7 kPa).
22 Particles can be separated in the following aerodynamic particle diameter ranges: <0.25;
23 0.25 to 0.5; 0.5 to 1.0; 1.0 to 2.5; and >2.5 μm . The collection substrates were 37 mm
24 PTFE filters (Pall) [in Prague](#) or quartz fibre filters (Pall) [in Barcelona](#) for the < 0.25 μm
25 [filter](#) stage, and 25 mm PTFE filters (Pall) for the 0.25-2.5 μm and >2.5 μm [impactor](#)
26 stages. Two of the PCIS deployed in Prague separated particle mass in all of the 5 size
27 fractions while another unit collected particles only at 3 of the stages (< 0.25 μm ; 0.25-2.5
28 μm and >2.5 μm). In order to facilitate interpretation of the data, a lower cut diameter of
29 30 nm was assumed for the last filter stage of particles < 0.25 μm (quasi-UFP).

30 All the cascade impactors were loaded with uncoated substrates to avoid possible
31 interferences in future chemical analysis (mainly, determination of organics), so the particle
32 bounce that might occur during dry collection has to be considered excepting for the case of

1 BLPI which foils were coated with a thin layer of vacuum grease (Apiezon L, Apiezon
2 products, M&I Materials Ltd, Manchester, England) to ensure adherence of deposited
3 particles and reduce the artefact of bounce.

4 For the Prague winter intercomparison, the abovementioned six different impactors were
5 deployed simultaneously in both outdoor and indoor sampling periods. The cascade impactors
6 and their inlets were positioned outside above the roof of ICPF building, 285 m.a.s.l. The
7 nano-Moudi, in order to protect its electrical components, was kept inside an air-conditioned
8 cabin with a temperature continually lower than 20°C and a metal pipe (about 300 cm long)
9 was extended through the roof of the building. With regard to indoor sampling, the impactors
10 were placed inside Laboratory of Aerosol Chemistry and Physics experimental hall on the 2nd
11 floor where office and other experimental activities take place. In both campaigns (indoor and
12 outdoor), the pump exhausts were extended far of the sampling spots in order to avoid
13 sampling artefacts.

14 For the Barcelona summer intercomparison, the same cascade impactors were deployed
15 (except for the PCIS) at the urban background monitoring site located in IDAEA-CSIC (78
16 m.a.s.l.; South West part of the city) within the University Campus and they were positioned
17 under a plastic shelter to protect them from rain while allowing free ventilation. All the
18 impactor pumps were placed 5 m distance from the impactors whilst long tubes (10 m) were
19 connected to the exhausts to avoid contamination of the samples.

20 The error in the sampling flow rate and sampled volume in both campaigns was < 5%. Thus,
21 it is assumed that flow rates did not affect the particle size cut-offs. The uncertainty in the
22 particle mass concentration determination was < 15% except in some cases for the smallest
23 stages of nano-BLPI and nano-Moudi impactor which reached mass value deviations > 20 %
24 (standard deviation).

25 The specifications of the campaigns and the impactors deployed in the intercomparison study
26 are summarized in Table 1. The BLPI was used as internal reference for the size distribution
27 in this study as it was calibrated with the method described by Hillamo and Kauppinen (1991)
28 for the fine stages and by Štefancová *et al.* (2011) for coarse stages. ~~For the intercomparison,
29 the modal pattern of aerosol mass size distribution was divided into four size groups: (i) PM₁₀
30 ($D_p < 10 \mu\text{m}$), (ii) PM₂ ($D_p < 2 \mu\text{m}$), (iii) PM₁ ($D_p < 1 \mu\text{m}$) and (iv) PM_{0.25} ($D_p < 0.25 \mu\text{m}$) particles.
31 Approximate lower cut points for those selected size fractions are shown in Table S2 in the
32 supplementary information.~~

1

2

Table 1. Impactors deployed in Prague and Barcelona and their specifications.

Impactor type	BLPI	nano-BLPI	nano-Moudi	PCIS (5 stages) ^c	PCIS (3 stages) ^d
Number of samplings in Prague	5x outdoor (3x weekend-days + 2x week-days) 2 x indoor (1xweekend-days + 1x week-days)	5x outdoor (3x weekend-days + 2x week-days) 2 x indoor (1xweekend-days + 1x week-days)	5x outdoor (3x weekend-days + 2x week-days) 2 x indoor (1xweekend-days + 1x week-days)	5x outdoor (3x weekend-days + 2x week-days) 2 x indoor (1xweekend-days + 1x week-days)	5x outdoor (3x weekend-days + 2x week-days) 2 x indoor (1xweekend-days + 1x week-days)
Number of samplings in Barcelona	4 x outdoor (4 x week-days)	4 x outdoor (4 x week-days)	4 x outdoor (4 x week-days)	N/A	N/A
Flow rate (L min ⁻¹) ^a	24.8	17.2	10	9	9
Sampling substrates	PET foils (MYLAR) 13 µm thick	PET foils (MYLAR) 13 µm thick	PTFE 47 mm	37 mm PTFE filters (Pall) < 0.25 µm stage and 25 mm PTFE filters (Pall) for the 0.25-2.5 µm and 2.5-10 µm stages	37 mm quartz-fibre filters (Pall) < 0.25 µm stage and 25 mm PTFE filters (Pall) for the 0.25-2.5 µm and >2.5 µm stages
N° Stages	10	8	13	5	3
Lower cut sizes (µm) ^b	0.026	0.011	0.01	0.03	0.03
	0.056	0.024	0.018	0.25	0.25
	0.10	0.039	0.032	0.50	2.50
	0.16	0.062	0.056	1.00	
	0.25	0.095	0.10	2.50	
	0.43	0.24	0.18		
	0.86	0.49	0.32		
	1.73	1.0	0.56		
	3.42		1.00		
	6.61		1.80		
			3.20		
			5.60		
			10		
Inlet cut-point (µm)	14	1.95	18	10	>2.5

3 ^a Volumetric flow rate at 20°C and ambient pressure4 ^b All sizes are aerodynamic equivalent diameters5 ^c Two units deployed; A cyclone was installed ahead which cut PM₁₀6 ^d One single unit deployed

7 N/A – Not available

8 **2.3 Sample conservation and gravimetric analysis**

9 Particle mass concentrations on impactor substrates were gravimetrically determined by pre-
10 and post-weighing the Mylar foils and filters (PTFE and quartz fiber) with a Sartorius M5P-
11 000V001 electronic microbalance in Prague and a Mettler MT5 electronic microbalance in
12 Barcelona, both with a ±1 µg sensitivity. Blank samples (1 per sample) were collected per
13 each impactor type in both intercomparison (Prague and Barcelona) for each of the sampling

1 periods. The deviation of mass values due to varying conditions was corrected with the help
2 of the corresponding blanks.

3 All samples were equilibrated for a period of 24 hours before weighing in a temperature and
4 relative humidity controlled room (20.0 ± 0.2 °C; 45.4 ± 0.6 % RH). The electrostatic charges
5 of the filters were removed using an U-shaped electrostatic neutralizer (Haug, type PRX U) in
6 Prague and a zerostat anti-static instrument (Z108812-1EA, Sigma-Aldrich Co. LLC.) in
7 Barcelona. Each sample was weighed three times with an accuracy of mass determination of ±
8 2 µg. After weighing, the sampled foils and filters were stored in the freezer at -18 °C.

9 **2.4 Ion chromatography analysis**

10 Ion chromatography analysis were only carried out for the Prague samples and for the BLPI,
11 nano-BLPI and nano-Moudi impactors with the aim to support the interpretation of the
12 particle mass size distributions data. The PCIS filters were not analysed due to the differences
13 observed for the finest size fraction with the other impactors, as will be discussed below.

14 The whole nano-Moudi impactor samples were extracted in 7 ml of ultrapure water. In case of
15 the Berner impactors, approximately 1/3 of each foil with samples from each stage was cut
16 out and number of aerosol spots on cut piece was calculated. The ratio between cut and total
17 number of spots at each impactor stage was used to recalculate results to overall ion amount
18 on each stage. All samples were then extracted with 7 ml of ultrapure water, sonicated for 30
19 min in ultrasonic bath and shaken for 1 hour using a shaker. The extracts were then analyzed
20 using a Dionex 5000 system both for cations (Na⁺, NH₄⁺, K⁺, Ca²⁺ and Mg²⁺) and anions
21 (SO₄²⁻, NO₃⁻, Cl⁻) in parallel. An IonPac AS11-HC 2 x 250 mm column was used for anions
22 using hydroxide eluent, IonPac CS18 2 x 250 mm for cations using methane sulfonic acid
23 solution as an eluent. Both anion and cation set-up were equipped with electrochemical
24 suppressors. External calibration was done using NIST traceable calibration solutions.

25 **3 Results**

26 **3.1 Meteorological data and mean aerosol concentrations in outdoor air**

27 Table 2 displays the meteorological data (ambient temperature, relative humidity, ambient
28 pressure and wind speed), the mean and standard deviations ($\pm\sigma$) of aerosol concentrations for
29 Prague and Barcelona and season during sampling with BLPI.

30

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24

Table 2. Meteorological data and mean daily aerosol concentrations in outdoor air in Prague from 6th to 23rd February 2015 and in in Barcelona from 18th May to 3rd July 2015.

Sampling site	Temperature (°C)		Relative humidity (RH, %)		Barometric pressure recalculated to sea level (mbar)	Wind Speed (km h ⁻¹)	Mean PM ₁₄ [±] (µg m ⁻³)
	Min	Max	Min	Max			
Prague (winter)	-3.4±2.6	3.9±3.3	51±15.4	92±2.1	1023±9.4	12.5±6.6	34.6 ± 15.8
Barcelona (summer)	18±3.3	26±3.3	39±9.9	85±7.1	1018±3.1	12±2.6	15.2 ± 2.1

During the winter campaign in outdoor air from 6th to 23rd February 2015 in Prague, the daily maximum average temperature was 3.9±3.3 °C and the minimum average temperature was -3.4±2.6 °C. The relative humidity varied in the range of 51-92% from day to day.

As expected, higher temperatures during summer were monitored in Barcelona from 18th May to 3rd July 2015 (minimum of 18±3 °C and maximum of 26±3 °C). However, slightly lower RH (minimum of 39±10 % and maximum of 85±7%), similar pressure (1018±3 mbar) and wind speed (12±3 km h⁻¹) values were recorded. The results imply that aqueous particles may have been collected on an impaction stage different from the stage where they ought to be collected due to the flow-induced relative humidity changes during the day (Fang *et al.*, 1991; Štefancová *et al.*, 2010). Aqueous particles can shrink due to evaporation caused by pressure drop through the impactor and/or grow due to condensation caused by aerodynamic cooling. Also, a distortion of the size distribution due to ~~bounce-off should not be neglected for Barcelona given that foils were not greased prior to sampling.~~ bounce-off should not be neglected for Barcelona in the nano-BLPI, nano-Moudi and PCIS given that foils were not greased prior to sampling. The same artefact is not expected to occur during winter in Prague (outdoors). This is supported by previous tests from BLPI (authors' unpublished data) showing no difference between two identical impactors when one of them used greased foils and the other one ungreased foils in winter conditions.

1 In Prague, the mean PM₁₄ mass concentration measured outdoors (with BLPI) was 34.6 ±
2 15.8 µg m⁻³ whilst in Barcelona (with BLPI) it was 15.2 ± 2.1 µg m⁻³ (Table 2), in a similar
3 order of magnitude than as during previous results from agreement with previous results from
4 2008 winter campaign in ICPF (Schwarz *et al.* 2012; PM₁₄=34 µg m⁻³) and of the same order
5 of magnitude as PM₁₀ from aduring a 2014 summer campaign in the monitoring station at
6 IDAEA-CSIC (PM₁₀=19.6 µg m⁻³). The reason of higher averages of particle mass
7 concentrations in winter in Prague than in summer in Barcelona are due to higher emissions
8 (mainly due to coal and biomass burning used for residential heating) and meteorological
9 conditions such as the lower mixing heights of the boundary layer or even temperature
10 inversions occurring in Prague (Schwarz *et al.*, 2012).

11 3.2 Average particle mass concentrations per stage for the different impactors

12 To estimate the cumulative mass concentration for the different size ranges in each of the
13 impactors, the integrated curve of the measured particle mass size distributions was
14 determined by Eq. 1:

$$15 \quad M_i = M_{i-1} + \int_{D_{pi-1}}^{D_{pi}} \frac{dM}{d \log D_p} \times d \log D_p \quad \text{Eq. (1)}$$

16 | Where, M_i is the estimated mass concentration for each impactor stage i , D_{pi-1} and D_{pi} are
17 respectively the lower and upper cut-off diameters of the impactor stage i

18 The cumulative curves of the particle mass size distributions from Prague (indoor and
19 outdoor) and Barcelona are shown in Figures 1 and 2, respectively.

20 Results show that the nano-BLPI behaved similarly to the internal reference considered for
21 this work (BLPI), especially for particles larger than 250 nm. Outdoors and indoors, the nano-
22 Moudi was in agreement with the BLPI for particles larger than 320 nm (independent of the
23 aerosol load and type). However, for particles below 320 nm, the particle mass concentration
24 of the nano-Moudi tended to be higher than for the BLPI, especially during winter in Prague.
25 In indoor air, the nano-Moudi cumulative curve of the mass size distributions was closer to
26 the curve obtained for the BLPI impactor.

27 While in Prague, the nano-Moudi mass size distributions for particles >1 µm were lower than
28 the rest of the impactors, in Barcelona, this trend was not so evident (Figure 1 and 2). This
29 different behaviour could be ascribed to a number of causes: (a) in outdoor air the effect of
30 particle bounce and/or the shrinkage of semi volatile compounds may have caused a shift in

1 particle mass towards the lower sizes of the nano-Moudi, especially in winter in Prague
2 resulting in higher concentrations for particles below 320 nm; and/or (b) indoors, the
3 mechanism of the nano-Moudi of spreading the sample (rotating plates) and also the heat
4 generated from the sensor board of nano-Moudi, with the increase in temperature, both in
5 indoor air and inside the nano-Moudi ~~shell~~cabinet, could favour particle
6 dissociation/evaporation from the PTFE filters and thus result in lower mass loads across the
7 lower size ranges, and thus the nano-Moudi curve would appear to be closer to the internal
8 reference BLPI. This effect would not be so prominent in outdoor air, given that the
9 instrument does not reach such temperature increments since it was kept inside an air-
10 conditioned cabin with a temperature continually lower than 20°C while indoors, the
11 temperature was continually higher than 23°C. For one sampling exercise outdoors, in Prague,
12 the instrument's temperature shown on nano-Moudi cabinet's screen increased from 18.8 °C
13 up to 26.6 °C after 4 hours sampling, and then increased up to 31.6 °C at the end of one of the
14 sampling periods (3 days sampling; 72h). The temperature increase (both indoors and
15 outdoors) was significant and able to explain dissociation of ammonium nitrate which
16 increases progressively with increasing temperature (Allen *et al.*, 1989; Stelson and Seinfeld,
17 1982; Talbot *et al.*, 2016). Ammonium chloride is known to behave similarly (Pio and
18 Harrison, 1987a,b; Allen *et al.*, 1989). Nie *et al.* (2010) also attributed the loss of volatile
19 compounds to the increase of the temperature inside the MOUDI.— However, nitrate
20 concentrations were low in indoor air (see sections below), and therefore the volatilization of
21 this species would have had a low impact on particle mass (leaving only the organic fraction
22 to account for this). Further research is necessary to clarify the different behaviours observed.

23 ~~The size fractionated average mass concentrations (PM_{0.25}, PM₁, PM₂ and PM₁₀) collected by~~
24 ~~each impactor along with standard errors deviation ($\pm\sigma$) in the respective size fractions, using~~
25 ~~data from a total of 5 experiments outdoors and 2 indoors in Prague, and a total of 4 valid~~
26 ~~samples outdoors in Barcelona are summarised in Figure 3. Approximate cut points for the~~
27 ~~selected size fractions are shown in Table S2 in the supporting information. However, it is~~
28 ~~important to take into account that some differences in the results could be partially attributed~~
29 ~~to the differences in the real cut points for the selected size fractions.~~


30 The average PM₁₄ mass concentrations and corresponding standard deviation obtained using
31 the internal reference (BLPI) -in Prague outdoors were $34.6 \pm 15.8 \mu\text{g m}^{-3}$. In Barcelona, the
32 PM₁₄ mass concentrations and standard deviation in summer were $15.2 \pm 2.1 \mu\text{g m}^{-3}$.

1 Comparison of independent data from Grimm laser spectrometer (corrected with high volume
2 samplingsampler) and the impactors with PM₁ and PM₁₀ size cuts, was carried out for the
3 outdoor campaign in Barcelona (4 samples). A slope of 0.98 and a R² of 0.7 was obtained for
4 the PM₁₄ for BLPI with PM₁₀ from an online laser spectrometer (corrected with regard to
5 reference instrumentation) whereas for PM₁, a slope of 0.7 and a better fit of the data was
6 obtained (R²=0.9). Similarly to BLPI, the nano-BLPI shows a slope of 0.7 and a R² of 1 for
7 the cut point PM₁. The mass differences detected for PM₁ suggest that impactors sampling
8 artefacts such as particle blow off, particle wall losses and/or particle bounce occurred.

9 Finally, the portable PCIS were only used in Prague during winter given the differences
10 obtained with regard to the BLPI for the quasi-ultrafine size mode (<250 nm; PM_{0.25}). A
11 similar pattern was observed for indoor air, although with a relatively smaller difference. A
12 possible reason for the discrepancies observed regarding the PM_{0.25} fraction could be ascribed
13 to the different pressure drops across the impactor stages originating from different flow rates
14 (e.g., PCIS 9 L min⁻¹ vs. BLPI 24.8 L min⁻¹). The higher pressure drop in the stationary
15 impactors (e.g., BLPI) may increase the probability of volatilisation of semi-volatile species
16 during prolonged sampling, and could contribute to an underestimation of the PM_{0.25} when
17 compared to the PCIS (Sioutas, 2004).

18 The differences with regard to the coarse fractions were much smaller when compared to the
19 quasi-UFP fractions. In outdoor air, the PCIS showed consistently higher concentrations for
20 particles larger than 1 µm. Similar results were reported by Sioutas (2004) where an average
21 ratio PCIS to Moudi (Model 110, MSP Corp, Minneapolis, MN) of 2.02 (± 0.59) and 1.21 (±
22 0.35) was reported for an aerodynamic size range < 0.25 µm and 2.5-1 µm, respectively.
23 However, in indoor air a consistently underestimation, was observed for an aerodynamic size
24 range 1-10 µm.


25 In summary, for the aerosols and sampling conditions in this work, the PCIS provided
26 comparable size-resolved mass concentrations for particles > 1 µm while the cut-off at 250
27 nm did not seem to be consistent with the internal reference BLPI. In order to fully
28 understand these phenomena, a more systematic evaluation might be required. For this reason,
29 data from PCIS will not be discussed in the following sections.

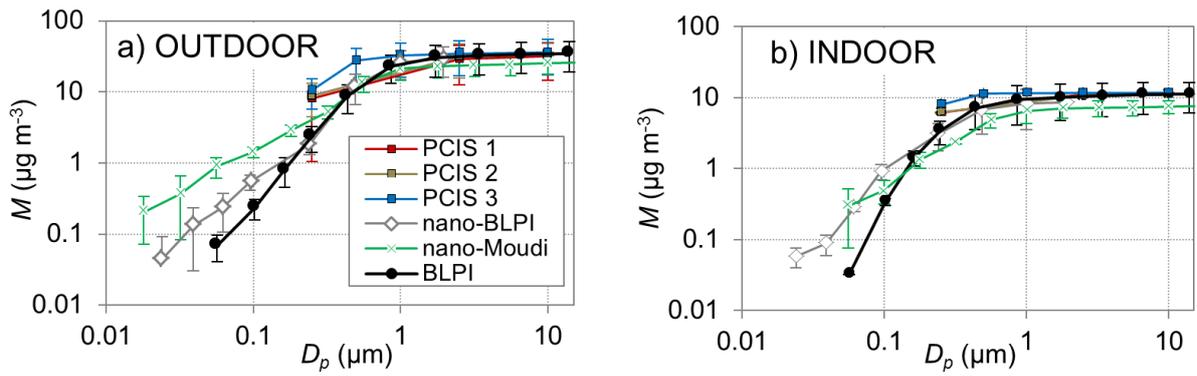

1

2 *Figure 1. Cumulative mass concentrations measured by the six impactors in Prague: (a)*
 3 *outdoors and (b) indoors. Error bars indicate the standard deviation ($\pm\sigma$).*

4

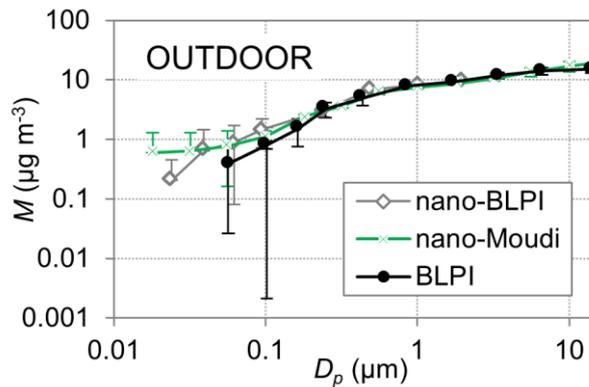

5

6 *Figure 2. Cumulative mass concentrations measured by the three impactors in Barcelona,*
 7 *outdoors. Error bars indicate the standard deviation ($\pm\sigma$).*

8 ~~As shown in Figure 3, the largest relative difference between the average mass concentrations~~
 9 ~~collected with the three impactors (PCIS, nano-BLPI and nano-Moudi) and the internal~~
 10 ~~reference (BLPI) was calculated for the $PM_{0.25}$ -size fraction measured outdoors in Prague by~~
 11 ~~PCIS and nano-Moudi, when concentrations were larger by 354 and 126 %, respectively. The~~
 12 ~~best agreement between the three impactors and the internal reference was obtained in the~~
 13 ~~Barcelona-summer-campaign.~~

14 ~~Interecomparisons between the nano-BLPI impactor and the reference BLPI indicate an overall~~
 15 ~~good agreement with absolute differences in mass concentrations per size fraction being~~
 16 ~~<30%, independent of the aerosol type. A consistent underestimation of the particle mass~~
 17 ~~concentrations for the $PM_{0.25}$ -size fractions was obtained with the nano-BLPI for all~~
 18 ~~campaigns and locations (Figure 3). This consistent underestimation was in the order of 5 and~~
 19 ~~22% outdoors in Barcelona and Prague, respectively, and 10% indoors in Prague, for $PM_{0.25}$ -~~

1 ~~As for PM₁, a slight overestimation of mass concentrations with regard to the BLPI was~~
2 ~~obtained by the nano-BLPI in both sampling campaigns outdoors. The largest deviation in this~~
3 ~~size fraction was obtained in Prague outdoors (15%) whereas the smallest difference was~~
4 ~~obtained in Barcelona (5%). Similar to the PM_{0.25} fraction, the PM₁ and PM₂ concentrations~~
5 ~~obtained indoors by the nano-BLPI were lower (12 and 15%, respectively) than those of the~~
6 ~~BLPI.~~

7 ~~As for the nano-Moudi, it consistently measured lower PM₁ and PM₂ concentrations in all~~
8 ~~campaigns (max difference obtained indoors for PM₁ = 31% and PM₂ = 30%). These~~
9 ~~differences can be explained by the difference in the cut points given that PM₁ and PM₂~~
10 ~~fractions from the BLPI are actually 0.86 μm and 1.7 μm, respectively. For quasi-UFP mass~~
11 ~~concentrations were significantly higher (126%) in Prague outdoors, whereas the~~
12 ~~disagreement with the BLPI was reduced in Barcelona outdoors (14%). Finally, in indoor air,~~
13 ~~concentrations registered by the nano-Moudi were lower (30%) than the BLPI, in Prague.~~

14 ~~Finally, the portable PCIS were only used in Prague during winter given the differences~~
15 ~~obtained with regard to the BLPI for the quasi-ultrafine size mode PM_{0.25} (354%). A similar~~
16 ~~pattern was observed for indoor air, although with a relatively smaller, but still high~~
17 ~~difference (75%). A possible reason for the discrepancies observed regarding the PM_{0.25}~~
18 ~~fraction could be ascribed to the different pressure drops across the impactor stages~~
19 ~~originating from different flow rates (e.g., PCIS 9 L min⁻¹ vs. BLPI 24.8 L min⁻¹). The higher~~
20 ~~pressure drop in the stationary impactors (e.g., BLPI) may increase the probability of~~
21 ~~volatilisation of semi-volatile species during prolonged sampling, and could contribute to an~~
22 ~~underestimation of the PM_{0.25} when compared to the PCIS (Sioutas, 2004).~~


23 ~~The differences with regard to the coarse fractions were much smaller when compared to the~~
24 ~~quasi-UFP fractions (<[±42%] and <[±27%] in outdoors and indoors, respectively). In~~
25 ~~outdoor air, the PCIS showed consistently higher PM₁, PM₂ and PM₁₀ concentrations (42, 14~~
26 ~~and 4%, respectively). Similar results were reported by Sioutas (2004) where an average ratio~~
27 ~~PCIS to Moudi (Model 110, MSP Corp, Minneapolis, MN) of 2.02 (± 0.59) and 1.21 (± 0.35)~~
28 ~~was reported for an aerodynamic size range < 0.25 μm and 2.5–10 μm, respectively. However,~~
29 ~~in indoor air a consistently underestimation (12, 16 and 21% for PM₁, PM₂ and PM₁₀), was~~
30 ~~observed.~~

~~In summary, for the aerosols and sampling conditions in this work, the PCIS provided comparable size-resolved mass concentrations for PM₄, PM₂ and PM₁₀ while the cut-off at 250 nm did not seem to be consistent with the internal reference BLPI. In order to fully understand these phenomena, a more systematic evaluation might be required. For this reason, data from PCIS will not be discussed in the following sections.~~

3.3 Aerosol mass size distributions

3.3.1 Particle size distribution in outdoor air

The average particle mass size distributions obtained in the outdoor intercomparison study (Prague and Barcelona) can be found in Figure 3.

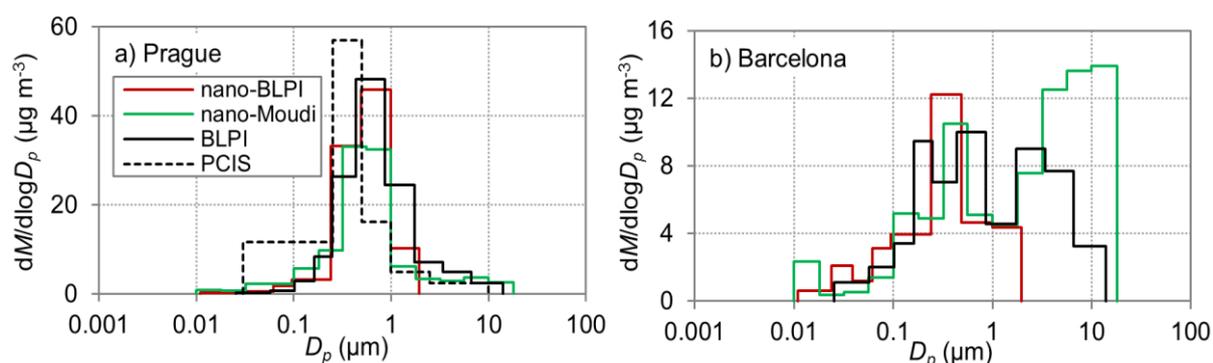

10

11 *Figure 3. Average mass size distributions obtained outdoors: (a) winter in Prague and (b)*
12 *summer in Barcelona.*

13 As can be seen, the particle mass size distributions are very different depending on the season
14 and sampling location. During winter in Prague (outdoors), the mass size distributions have a
15 predominantly fine mode, with the coarse mode being almost negligible (by all impactors).
16 The maximum mass concentration obtained in the fine size fraction mode was between 0.4-
17 0.9 μm , whereas in summer in Barcelona, this maximum was shifted towards smaller size
18 fractions between 0.2 and 0.4 μm . In addition to the different aerosol types, this shift to lower
19 sizes might be caused by a lower average relative humidity during sampling in Barcelona that
20 could have caused the particle drying (Tables 2) and therefore, be a reason for particle bounce
21 (Fang *et al.*, 1991; Štefancová *et al.*, 2010). In Prague (outdoors), particle bounce had a
22 negligible effect because high RH was recorded. This is important~~In the same time~~
23 as only few coarse particles were present and at the same time the high share of primary, less
24 oxygenated organics was found (Kubelová *et al.*, 2015; Vodička *et al.*, 2013). Although it is

1 ~~known that RH is lowered at each stage of any cascade impactor due to kinetic effects and to~~
2 ~~short time of flight between the nozzle and the impaction plate, this decrease is only moderate~~
3 ~~for the first stages. For example, the pressure below stage 6 of the BLPI which corresponds to~~
4 ~~particles as smaller than 440 nm is only 6% lower than ambient. A similar value is found~~
5 ~~for nano-BLPI for equivalent stage. The nano-Moudi has even smaller pressure drops at~~
6 ~~equivalent stages. The drying becomes important for lower stages, however~~ Indeed, it is
7 ~~known that kinetic effect limiting drying of particles would be more pronounced at lower~~
8 ~~temperatures in winter due to lower equilibrium water vapor pressure, and drying of particles~~
9 ~~can occur. In any case, atmospheric particles in this size range below 250 nm are comprised~~
10 ~~mostly of organics, especially in winter (see e.g Kubelová *et al*, 2015). These fractions of~~
11 ~~organics are often of semiliquid nature and this fact efficiently prevents bounce.~~

12 While in Prague during winter the coarse mode was mostly insignificant, in Barcelona during
13 summer the mass size distributions were clearly bimodal, with larger coarse mode
14 concentrations (Figure 3). The coarse mode obtained may be due to mineral and marine
15 aerosol contributions in the study area (Querol *et al.*, 2008).

16 The majority of mass concentrations were found in the accumulation mode (PM₁) for both
17 campaigns ($7.9 \pm 0.7 \mu\text{g m}^{-3}$ and $22.9 \pm 9.8 \mu\text{g m}^{-3}$ according the internal reference BLPI in
18 summer Barcelona and winter Prague, respectively). With the increase in mass there was an
19 increase in agreement between the impactors, where the closest agreement was observed
20 (between 200-600 nm) (Figure 3).

21 Figure 3 reveals that the nano-Moudi recorded higher particle mass concentrations in the
22 ultrafine range (<100 nm) than the reference BLPI during winter in Prague (5 samples in total
23 outdoors). Although differences were smaller, the same is true for the Barcelona summer
24 campaign (~~4-week sampling~~ 4 samples in total, Figure 3). As previously mentioned, to protect
25 the electrical components of the nano-Moudi during winter campaign in Prague outdoors, it
26 was kept inside a climate controlled cabin with a temperature continually lower than 20°C. At
27 these temperatures dissociation of ammonium nitrate can still occur at a slow rate (Smolík *et*
28 *al.*, 2008). In addition, during the sampling, an increase of temperature inside the nano-Moudi
29 ~~shell-cabinet~~ was detected due to the internal mechanism of spreading the sample (rotating
30 plates) ~~and the electric current in the sensor board~~ which generates heat. It is therefore likely
31 that the internal temperature in the nano-Moudi (~~always >30 °C~~) was higher than that of the
32 cabin (~~<20 °C~~) and thus led to particle volatilisation (Štefancová *et al.*, 2010). The lower


1 nitrate and chloride concentrations in the accumulation mode on the nano-Moudi filters (see
2 below) would support this interpretation. It is also known that a 5°C difference between the
3 PTFE filter (of the type used in the nano-Moudi) and sampling temperature may accelerate
4 the dissociation of ammonium nitrate on PTFE filters up to 20% (Hering and Cass, 1999).
5 The BLPI and nano-BLPI have no internal warming mechanisms and were located outdoors
6 in Prague and Barcelona, so it is expected that lower volatilisation would occur in these
7 scenarios. However, drying of particles before they are deposited on a substrate may happen
8 also in the BLPI and nano-BLPI due to ~~lower residence time and~~ higher pressure drops (at
9 equivalent sizes) ~~and despite lower residence times~~ in comparison with the nano-Moudi. This
10 would increase the driving force for evaporation at those stages, which would encourage
11 particle shrinkage. However the situation is more complicated while a particle is incorporated
12 into a deposit of particles where other processes like diffusion in semiliquid mixture of other
13 organics or Raoult's law play their roles. This process anyhow influences the measured
14 concentrations and therefore the impactors comparison.
15 Furthermore, decomposition of ammonium nitrate and chloride, is probably also enhanced in
16 the nano-Moudi due to the spreading of the sample on the whole filter surface, in comparison
17 with thick individual spots of material obtained with the BLPI and nano-BLPI impactors. All
18 these previous facts (temperature, RH, high surface area) appear to enhance the evaporation of
19 semi-volatiles (and dissociation of ammonium nitrate) and therefore particle shrinkage during
20 transport through the nano-Moudi explaining the mass size distributions from the nano-Moudi
21 being skewed towards smaller particle fractions during the Barcelona and Prague campaigns
22 (Figure 3). Also, the residence time of particles inside the nano-Moudi low pressure stages is
23 longer due to the lower volumetric flow rate in this instrument. All of this could thus explain
24 the mass size distributions from the nano-Moudi being skewed towards smaller particle
25 fractions during the Barcelona and Prague campaigns (Figure 3). It should be stated that the
26 rotation of the impaction plates and the nozzle plates of the nano-Moudi was specifically
27 designed to achieve a uniform deposit on the collection substrates and therefore, eradicate the
28 particle bounce-off artefact (Marple *et al.*, 2014) that may otherwise occur. Particle bounce-
29 off would only be expected when collecting particles in dry conditions such as in Barcelona
30 (< 50% RH) (Table 2) or indoors. Finally, the overall internal volumes in the low pressure
31 stages seem similar in all of the impactors tested; however, this would need experimental
32 confirmation.

1 3.3.2 Particle size distribution in indoor air

2 In Prague, indoor concentrations were lower than outdoors mainly due to a change in weather
3 conditions resulting in cleaner air masses during sampling periods (Figure 3 and Figure 4).
4 Reduced penetration efficiency and faster settling times probably explain the lower indoor
5 coarse mode mass obtained (Figure 4; Hussein *et al.*, 2007). Once again, the nano-BLPI
6 measured similar mass concentrations to the reference BLPI while the nano-Moudi recorded
7 notably lower mass from fine to coarse modes. In addition, the nano-Moudi size distribution
8 showed a slight shift towards larger particle sizes (Figure 4). The difference between the
9 BLPIs and the nano-Moudi could suggest that the latter underestimated mass during this
10 campaign for all particle cut sizes. Initially this would appear to reduce the possibility of
11 volatility losses being responsible for this difference, as ammonium nitrate dissociates readily
12 indoors thereby causing equal losses to all impactors (Lunden *et al.*, 2003). However, because
13 of the way the sample is spread across the substrate in the nano-Moudi, as described above,
14 the ammonium nitrate collected would be more prone to volatilization than that collected on
15 the other impactors. Therefore it could be considered that the mechanism of the nano-Moudi
16 of spreading the sample (rotating plates), with the increase in temperatures, both indoors and
17 inside the nano-Moudi ~~shell~~cabinet, could enhance dissociation/evaporation from the nano-
18 Moudi PTFE substrates. This conclusion can be supported by Figures 5 and 6, which show
19 significantly lower mass concentrations of major species of ammonium nitrate with the nano-
20 Moudi, in comparison with the BLPI.

21 A number of sources of uncertainty in this interpretation should be taken into account:

- 22 a) Increased uncertainty in the mass determination due to lower mass concentrations and
23 shorter sampling times
- 24 b) No blank correction available for nano-Moudi IC data
- 25 c) No uncertainty calculations for mass determinations available for nano-Moudi,
26 possibly resulting in negative mass concentrations in the lower stages
- 27 d) Only 2 valid samples available for indoor air (for all impactors)

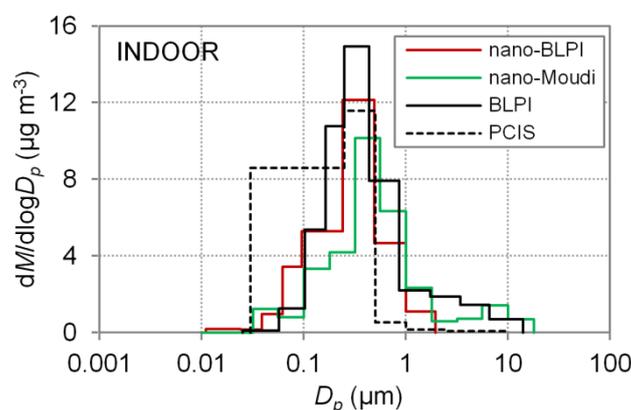

1

2 *Figure 4. Average mass size distributions in Prague during winter in indoor air.*


3 **3.3.3 Size distribution of inorganic ions**

4 Figures 5 and 6 show the particle mass size distributions of major (SO_4^{2-} , NO_3^- and NH_4^+) and
 5 minor (Cl^- , Na^+ , K^+ , Mg^{2+} and Ca^{2+}) aerosol constituents for the winter campaign in Prague in
 6 outdoor and indoor air, respectively. Corresponding actual mean values for mass concentra-
 7 tions for all of the ions analyzed for each of the environments (indoor and outdoor) in Prague,
 8 are shown in Table S2 of the supplementary information. The uncertainty of the blanks is also
 9 included in the Table S2.

10 In the winter in Prague, the mass size distributions of components have a predominantly fine
 11 mode ($< 1 \mu\text{m}$), with the coarse mode being almost negligible in winter in Prague (by all
 12 impactors) but highly significant in Barcelona during summer, such as the case for BLPI.


13 While the fine mode was dominant for the particle mass concentration and all the
 14 predominant aerosol constituents (SO_4^{2-} , NO_3^- and NH_4^+) for both indoor and outdoor air
 15 during winter in Prague, the average mass size distributions for minor species (Cl^- , Na^+ , K^+ ,
 16 Mg^{2+} and Ca^{2+}), were clearly multimodal (Figures 5 and 6). Similar mass size distributions of
 17 these species were obtained by the nano-BLPI and the reference BLPI both outdoors and
 18 indoors in Prague. However marked differences in the mass size distributions of these species
 19 were observed with the nano-Moudi. In outdoor air there is a clear decrease of NO_3^-
 20 ~~and NH_4^+~~ -concentrations measured with the nano-Moudi ($\text{PM}_{10} = 1.7 \mu\text{g m}^{-3}$; Table S2),
 21 confirming the interpretations provided in the previous sections. The same is valid for fine
 22 chlorides that are missing on same nano-Moudi samples showing ammonium chloride
 23 evaporation (NH_4Cl). Nitrates present indoors (due to indoor ammonium nitrate dissociation;
 24 Allen *et al.*, 1989; Stelson and Seinfeld, 1982; Talbot *et al.*, 2016) are influenced by other

1 species different to ammonium salts (e.g. sodium or potassium nitrate) that are not prone to
2 dissociation. For this reason, the difference between nano-Moudi and the other impactors
3 indoors (Figure 6) was much smaller compared to outdoors (Figure 5). The lower sulphate
4 and mass concentration on nano-Moudi indoor samples were caused by other factors (possibly
5 bounce) given that average RH indoors in winter was low (21%). In addition, outdoors in
6 Prague, the mass size distributions obtained by the BLPI showed that Ca^{2+} , Na^+ and Mg^{2+}
7 were dominated by coarse modes and for the case of K^+ , the fine mode is the dominant one
8 (suggesting biomass combustion as a possible emission source). As for Cl^- , the mass size
9 distributions were clearly bimodal. The nano-Moudi outdoors had different size distributions
10 from the BLPI for Cl^- , Na^+ , Ca^{2+} and Mg^{2+} . Only for K^+ the size distribution is similar. Mass
11 size distributions of Cl^- and Na^+ may have been influenced by filter contamination. The Ca^{2+}
12 peak detected at around 100 nm obtained by the nano-BLPI in outdoor air may possibly be
13 ascribed also to filter contamination, although no specific data are available to support this
14 interpretation. Similar peaks at 10 and 50 nm were observed indoors with the nano-Moudi and
15 nano-BLPI which may suggest bounce, contamination or blank variability.

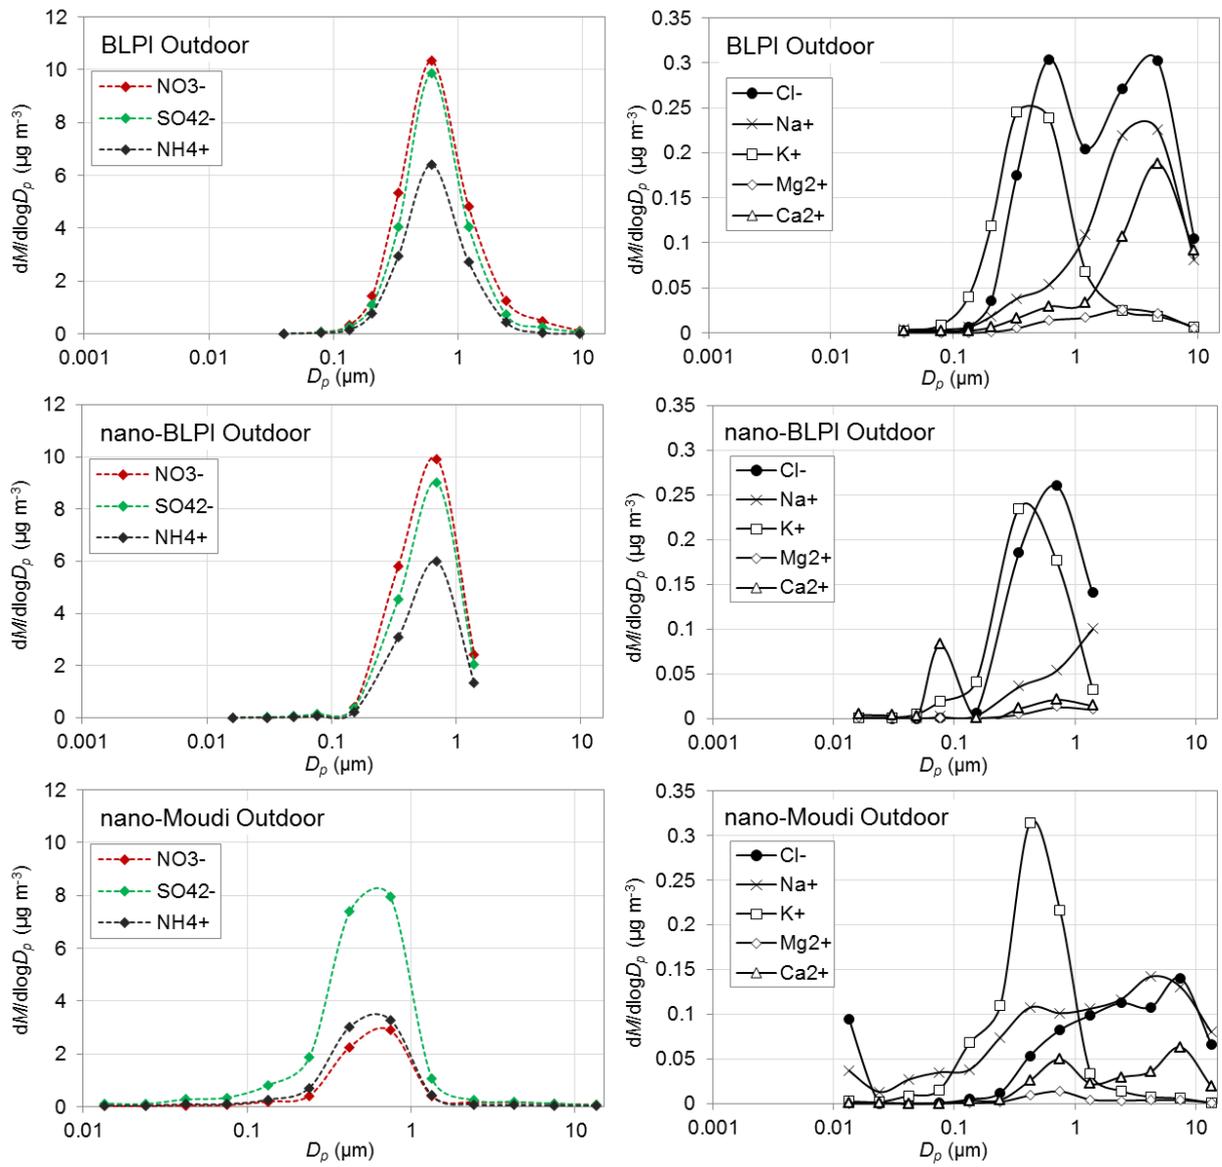

1

2 Figure 5. Average mass size distributions for different ionic species (left: SO_4^{2-} , NO_3^- and
 3 NH_4^+ and right: Cl^- , Na^+ , K^+ , Mg^{2+} and Ca^{2+}) during winter in outdoor air in Prague.

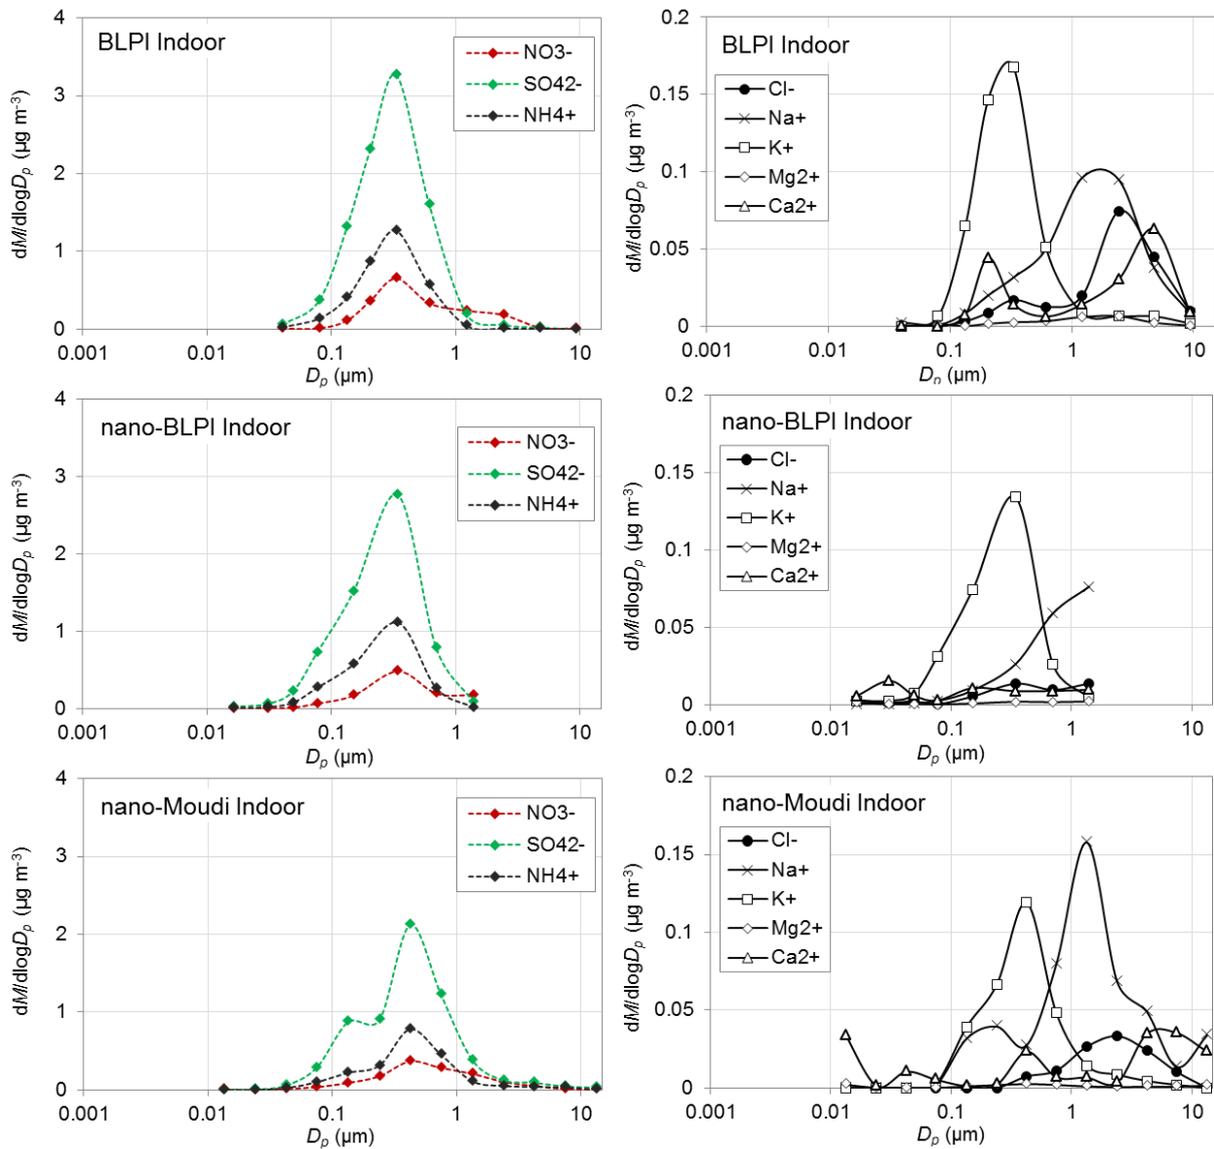

1

2 *Figure 6. Average mass size distributions for different ionic species (left: SO_4^{2-} , NO_3^- and*
 3 *NH_4^+ and right: Cl^- , Na^+ , K^+ , Mg^{2+} and Ca^{2+}) during winter in indoor air in Prague.*

4 **4 Conclusions**

5 This work aimed to assess the performance of four conventional and nano-range impactors,
 6 by means of two intercomparison exercises in Prague, during winter 2015 and in Barcelona
 7 during summer 2015. The aim of the campaigns was to test the instruments' performance with
 8 regard to the particle mass size distributions under different aerosol compositions resulting
 9 from different emission sources, meteorology, seasons, and air mass origins. All the cascade
 10 impactors were loaded with uncoated substrates excepting for the case of BLPI which foils
 11 were coated.

1 Taking the BLPI as an internal reference, the best agreement regarding mass size distributions
2 was obtained with the nano-BLPI, especially for particles larger than 250 nm. The nano-
3 Moudi showed a good agreement for particle sizes >320 nm, whereas for particle diameters
4 <320 nm this instrument recorded larger mass concentrations than the internal reference.
5 Different particle effects may have caused the differences regarding particle mass
6 concentrations collected in indoor and outdoor air by the nano-Moudi. Particle volatilisation
7 may have occurred due to the internal rotating mechanisms and the electric current in the
8 sensor board of nano-Moudi which heat the impactor casing up. Decomposition of
9 ammonium nitrate and chloride, as evidenced by the lower nitrate and chloride concentrations
10 in the accumulation mode, is probably also enhanced in the nano-Moudi due to the spreading
11 of the sample on the whole filter surface, in comparison with thick individual spots of
12 material obtained with the BLPI and nano-BLPI impactors. Further research is needed to
13 clarify this issue. With regard to the PCIS, their size-resolved mass concentrations were
14 comparable with other impactors ~~for PM₁, PM₂ and PM₁₀~~, but the cut-off at 0.25 µm was not
15 consistent with that of the internal reference.

16 In Barcelona, the sampling took place under dry conditions (< 50% RH) and thus, particle
17 bounce would be expected since some particles (depending on composition) could get dry.
18 Inversely, bounce can be probably neglected for the Prague outdoor intercomparison since the
19 RH was always >50 % indicating the presence of droplet aerosols that tend to adhere to the
20 impaction substrate. ~~To avoid such an effect impactor substrates should always be greased~~
21 ~~especially in areas with low humidity.~~

22 Aerosol mass size distributions were assessed for the Prague and Barcelona campaigns.
23 During winter in Prague (outdoors), the mass size distributions showed a predominantly fine
24 mode, with the coarse mode being almost negligible (by all impactors). However, in
25 Barcelona, the coarse size fractions showed larger mass concentrations, evidencing the higher
26 influence of mineral and marine aerosols.

27 This study concludes that comparability between the different types of impactors assessed
28 was dependent on particle size. Different performances when challenged with secondary
29 aerosols (due to volatilization) with regard to primary aerosols (potential bounce, also
30 affecting secondary inorganics), were observed. Specifically, the influence of the
31 differences in impactor construction (number of jets, flow, vapour pressure, etc.) on UFP
32 mass concentrations should be further addressed. In addition, further research is necessary

1 with regard to the particle processes (evaporation, bounce, etc.) behind the differences in
2 particle mass observed across size fractions in this study.

3 The conclusions from this work allow us to extract the following recommendations with re-
4 gard to ultrafine particle sampling with cascade impactors:

- 5 ▪ To avoid particle bounce and increase the accuracy of the size cuts, impactor substrates
6 should be greased especially in areas and seasons with low humidity.
- 7 ▪ Detailed assessments of the sampling duration should be carried out to allow sufficient
8 collection of material on each stage for adequate quantification without overloading the
9 upper collection stages. Common approaches to avoid particle overloading include using
10 multiple-orifice collection stages, and rotating collection substrates (Marple et al., 2014;
11 Marple et al., 1991).
- 12 ▪ Attention should be paid to volatilization issues during aerosol transport inside the im-
13 pactors especially with regard to temperature increases associated with internal rotating
14 mechanisms and the electric current in the sensor board of nano-Moudi.
- 15 ▪ Attention should also be paid to sample storage, to avoid evaporation of already deposited
16 particles that may lead to a decrease of mass on a given stage. This evaporation would
17 modify the observed aerosol size distribution, and would affect all impactor types.

18 **Acknowledgements**

19 The research leading to these results received funding from the European Community's
20 Seventh Framework Program (FP7-PEOPLE-2012-ITN) no. 315760 (HEXACOMM project).
21 It was also supported by Charles University in Prague, under the project GA UK no. 274213
22 and the Spanish MINECO, under the frame of SIINN, the ERA-NET for a Safe
23 Implementation of Innovative Nanoscience and Nanotechnology, in the framework of
24 ERANET-SIINN project CERASAFE (id.:16).

25 **References**

- 26 Allen, A.G., Harrison, R.M., Erisman, J.-W. (1989). Field measurements of the dissociation
27 of ammonium nitrate and ammonium chloride aerosols. *Atmospheric Environment*
28 (1967), 23(7), 1591-1599. doi: [http://dx.doi.org/10.1016/0004-6981\(89\)90418-6](http://dx.doi.org/10.1016/0004-6981(89)90418-6)
- 29 Amato, F., Alastuey, A., Karanasiou, A., Lucarelli, F., Nava, S., Calzolari, G., Severi, M.,
30 Becagli, S., Gianelle, V.L., Colombi, C., Alves, C., Custódio, D., Nunes, T.,
31 Cerqueira, M., Pio, C., Eleftheriadis, K., Diapouli, E., Reche, C., Minguillón, M.C.,

- 1 Manousakas, M., Maggos, T., Vratolis, S., Harrison, R.M., Querol, X. (2015).
2 AIRUSE-LIFE+: a harmonized PM speciation and source apportionment in 5
3 Southern European cities. *Atmos. Chem. Phys. Discuss.*, 15(17), 23989-24039. doi:
4 10.5194/acpd-15-23989-2015
- 5 BcnMap. (2015). Barcelona Map, Ajuntament de Barcelona, from
6 http://w20.bcn.cat/Guiamap/Default_en.aspx#x=27601.01&y=83987.71&z=0&w=980
7 [http://w20.bcn.cat/Guiamap/Default_en.aspx#x=27601.01&y=83987.71&z=0&w=980](http://w20.bcn.cat/Guiamap/Default_en.aspx#x=27601.01&y=83987.71&z=0&w=980&h=574&base=GuiaMartorell)
8 Berner, A., Luerzer, C. (1980). Mass size distributions of traffic aerosols at Vienna. *The*
9 *Journal of Physical Chemistry*, 84(16), 2079-2083. doi: 10.1021/j100453a016
- 10 Berner, A., Lürzer, C., Pohl, F., Preining, O., Wagner, P. (1979). The size distribution of the
11 urban aerosol in Vienna. *Science of The Total Environment*, 13(3), 245-261. doi:
12 [http://dx.doi.org/10.1016/0048-9697\(79\)90105-0](http://dx.doi.org/10.1016/0048-9697(79)90105-0)
- 13 Biswas, P., Flagan, R.C. (1984). High-velocity inertial impactors. *Environmental Science &*
14 *Technology*, 18(8), 611-616. doi: 10.1021/es00126a009
- 15 Crilley, L.R., Ayoko, G.A., Jayaratne, E.R., Salimi, F., Morawska, L. (2013). Aerosol mass
16 spectrometric analysis of the chemical composition of non-refractory PM1 samples
17 from school environments in Brisbane, Australia. *Science of The Total Environment*,
18 458-460, 81-89. doi: <http://dx.doi.org/10.1016/j.scitotenv.2013.04.007>
- 19 Delgado-Saborit, J.M., Stark, C., Harrison, R.M. (2014). Use of a versatile high efficiency
20 multiparallel denuder for the sampling of PAHs in ambient air: gas and particle phase
21 concentrations, particle size distribution and artifact formation. [Research Support,
22 Non-U S Gov't]. *Environ Sci Technol*, 48(1), 499-507.
- 23 Fang, C.P., McMurry, P.H., Marple, V.A., Rubow, K.L. (1991). Effect of Flow-induced
24 Relative Humidity Changes on Size Cuts for Sulfuric Acid Droplets in the
25 Microorifice Uniform Deposit Impactor (MOUDI). *Aerosol Science and Technology*,
26 14(2), 266-277. doi: 10.1080/02786829108959489
- 27 Fujitani, Y., Hasegawa, S., Fushimi, A., Kondo, Y., Tanabe, K., Kobayashi, S., Kobayashi, T.
28 (2006). Collection characteristics of low-pressure impactors with various impaction
29 substrate materials. *Atmospheric Environment*, 40(18), 3221-3229. doi:
30 <http://dx.doi.org/10.1016/j.atmosenv.2006.02.001>
- 31 Geller, M.D., Kim, S., Misra, C., Sioutas, C., Olson, B.A., Marple, V.A. (2002). A
32 Methodology for Measuring Size-Dependent Chemical Composition of Ultrafine
33 Particles. *Aerosol Science and Technology*, 36(6), 748-762. doi:
34 10.1080/02786820290038447
- 35 Hering, S., Cass, G. (1999). The Magnitude of Bias in the Measurement of PM_{2.5} Arising
36 from Volatilization of Particulate Nitrate from Teflon Filters. *Journal of the Air &*
37 *Waste Management Association*, 49(6), 725-733. doi:
38 10.1080/10473289.1999.10463843
- 39 Hering, S.V., Flagan, R.C., Friedlander, S.K. (1978). Design and evaluation of new low-
40 pressure impactor. I. *Environmental Science & Technology*, 12(6), 667-673. doi:
41 10.1021/es60142a004
- 42 Hillamo, R.E., Kauppinen, E.I. (1991). On the Performance of the Berner Low Pressure
43 Impactor. *Aerosol Science and Technology*, 14(1), 33-47. doi:
44 10.1080/02786829108959469
- 45 Hinds, W.C. (1999). *Aerosol technology : properties, behavior, and measurement of airborne*
46 *particles*. New York: Wiley.
- 47 Hitzengerger, R., Berner, A., Galambos, Z., Maenhaut, W., Cafmeyer, J., Schwarz, J., Müller,
48 K., Spindler, G., Wieprecht, W., Acker, K., Hillamo, R., Mäkelä, T. (2004).
49 Intercomparison of methods to measure the mass concentration of the atmospheric

1 aerosol during INTERCOMP2000-influence of instrumentation and size cuts.
2 *Atmospheric Environment*, 38(38), 6467-6476. doi:
3 <http://dx.doi.org/10.1016/j.atmosenv.2004.08.025>

4 Howell, S., Pszenny, A.A.P., Quinn, P., Huebert, B. (1998). A Field Intercomparison of Three
5 Cascade Impactors. *Aerosol Science and Technology*, 29(6), 475-492. doi:
6 10.1080/02786829808965585

7 Huang, Z., Harrison, R.M., Allen, A.G., James, J.D., Tilling, R.M., Yin, J. (2004). Field
8 intercomparison of filter pack and impactor sampling for aerosol nitrate, ammonium,
9 and sulphate at coastal and inland sites. *Atmospheric Research*, 71(3), 215-232. doi:
10 <http://dx.doi.org/10.1016/j.atmosres.2004.05.002>

11 Hussein, T., Glytsos, T., Ondráček, J., Dohányosová, P., Ždímal, V., Hämeri, K., Lazaridis,
12 M., Smolík, J., Kulmala, M. (2006). Particle size characterization and emission rates
13 during indoor activities in a house. *Atmospheric Environment*, 40(23), 4285-4307. doi:
14 <http://dx.doi.org/10.1016/j.atmosenv.2006.03.053>

15 Hussein, T., Kukkonen, J., Korhonen, H., Pohjola, M., Pirjola, L., Wraith, D., Härkönen, J.,
16 Teinilä, K., Koponen, I.K., Karppinen, A., Hillamo, R., Kulmala, M. (2007).
17 Evaluation and modeling of the size fractionated aerosol particle number
18 concentration measurements nearby a major road in Helsinki – Part II: Aerosol
19 measurements within the SAPPHIRE project. *Atmos. Chem. Phys.*, 7(15), 4081-4094.
20 doi: 10.5194/acp-7-4081-2007

21 IPR. (2015). Geoportal Praha, Prague geographic data in one place, Prague Institute of
22 Planning and Development (IPR Praha), from [http://www.geoportalpraha.cz/en/maps-](http://www.geoportalpraha.cz/en/maps-online#.VIIWWLerR1s)
23 [online#.VIIWWLerR1s](http://www.geoportalpraha.cz/en/maps-online#.VIIWWLerR1s)

24 Jiménez, S., Ballester, J. (2011). Use of a Berner Low-Pressure Impactor at Low Inlet
25 Pressures. Application to the Study of Aerosols and Vapors at High Temperature.
26 *Aerosol Science and Technology*, 45(7), 861-871. doi:
27 10.1080/02786826.2011.566900

28 Karanasiou, A.A., Sitaras, I.E., Siskos, P.A., Eleftheriadis, K. (2007). Size distribution and
29 sources of trace metals and n-alkanes in the Athens urban aerosol during summer.
30 *Atmospheric Environment*, 41(11), 2368-2381. doi:
31 <http://dx.doi.org/10.1016/j.atmosenv.2006.11.006>

32 Kubelová, L., Vodička, P., Schwarz, J., Cusack, M., Makeš, O., Ondráček, J., Ždímal, V.
33 (2015). A study of summer and winter highly time-resolved submicron aerosol
34 composition measured at a suburban site in Prague. *Atmospheric Environment*, 118,
35 45-57. doi: <http://dx.doi.org/10.1016/j.atmosenv.2015.07.030>

36 Lin, C.-C., Chen, S.-J., Huang, K.-L., Hwang, W.-I., Chang-Chien, G.-P., Lin, W.-Y. (2005).
37 Characteristics of Metals in Nano/Ultrafine/Fine/Coarse Particles Collected Beside a
38 Heavily Trafficked Road. *Environmental Science & Technology*, 39(21), 8113-8122.
39 doi: 10.1021/es048182a

40 Lunden, M.M., Revzan, K.L., Fischer, M.L., Thatcher, T.L., Littlejohn, D., Hering, S.V.,
41 Brown, N.J. (2003). The transformation of outdoor ammonium nitrate aerosols in the
42 indoor environment. *Atmospheric Environment*, 37(39-40), 5633-5644. doi:
43 <http://dx.doi.org/10.1016/j.atmosenv.2003.09.035>

44 Marple, V., Olson, B., Romay, F., Hudak, G., Geerts, S.M., Lundgren, D. (2014). Second
45 Generation Micro-Orifice Uniform Deposit Impactor, 120 MOUDI-II: Design,
46 Evaluation, and Application to Long-Term Ambient Sampling. *Aerosol Science and*
47 *Technology*, 48(4), 427-433. doi: 10.1080/02786826.2014.884274

- 1 Marple, V.A., Rubow, K.L., Behm, S.M. (1991). A Microorifice Uniform Deposit Impactor
2 (MOUDI): Description, Calibration, and Use. *Aerosol Science and Technology*, 14(4),
3 434-446. doi: 10.1080/02786829108959504
- 4 Mašková, L., Smolík, J., Vodička, P. (2015). Characterisation of particulate matter in
5 different types of archives. *Atmospheric Environment*, 107, 217-224. doi:
6 <http://dx.doi.org/10.1016/j.atmosenv.2015.02.049>
- 7 May, K.R. (1945). The Cascade Impactor. *Journal of Scientific Instruments*, 22(12), 247.
- 8 Misra, C., Singh, M., Shen, S., Sioutas, C., Hall, P.M. (2002). Development and evaluation of
9 a personal cascade impactor sampler (PCIS). *Journal of Aerosol Science*, 33(7), 1027-
10 1047. doi: 10.1016/s0021-8502(02)00055-1
- 11 Nie, W., Wang, T., Gao, X., Pathak, R.K., Wang, X., Gao, R., Zhang, Q., Yang, L., Wang, W.
12 (2010). Comparison among filter-based, impactor-based and continuous techniques for
13 measuring atmospheric fine sulfate and nitrate. *Atmospheric Environment*, 44(35),
14 4396-4403. doi: <http://dx.doi.org/10.1016/j.atmosenv.2010.07.047>
- 15 Oberdörster, G. (2000). Pulmonary effects of inhaled ultrafine particles. *Int Arch Occup*
16 *Environ Health*, 74(1), 1-8. doi: 10.1007/s004200000185
- 17 Oberdorster, G., Oberdorster, E., Oberdorster, J. (2005). Nanotoxicology: an emerging
18 discipline evolving from studies of ultrafine particles. *Environ Health Perspect*,
19 113(7), 823-839.
- 20 Ondráček, J., Schwarz, J., Ždímal, V., Andělová, L., Vodička, P., Bízek, V., Tsai, C.J., Chen,
21 S.C., Smolík, J. (2011). Contribution of the road traffic to air pollution in the Prague
22 city (busy speedway and suburban crossroads). *Atmospheric Environment*, 45(29),
23 5090-5100. doi: <http://dx.doi.org/10.1016/j.atmosenv.2011.06.036>
- 24 Pennanen, A.S., Sillanpaa, M., Hillamo, R., Quass, U., John, A.C., Branis, M., Hunova, I.,
25 Meliefste, K., Janssen, N.A., Koskentalo, T., Castano-Vinyals, G., Bouso, L., Chalbot,
26 M.C., Kavouras, I.G., Salonen, R.O. (2007). Performance of a high-volume cascade
27 impactor in six European urban environments: mass measurement and chemical
28 characterization of size-segregated particulate samples. *Sci Total Environ*, 374(2-3),
29 297-310.
- 30 Pio, C.A. and Harrison, R.M. (1987a). The equilibrium of ammonium chloride aerosol with
31 gaseous hydrochloric acid and ammonia under tropospheric conditions. *Atmospheric*
32 *Environment*, 21, 1243-1246.
- 33 Pio, C.A. and Harrison, R.M. (1987b). Vapour Pressure of ammonium chloride aerosol..
34 Effect of temperature and humidity. *Atmospheric Environment*, 21, 2711-2715.
- 35 Preining, O., Berner, A. (1979). Aerosol Measurements in the Submicron Size Range. *EPA*
36 *report, EPA-600/2-79-105*. Washington, DC: EPA.
- 37 Querol, X., Alastuey, A., Moreno, T., Viana, M.M., Castillo, S., Pey, J., Rodríguez, S.,
38 Artiñano, B., Salvador, P., Sánchez, M., Garcia Dos Santos, S., Herce Garraleta, M.D.,
39 Fernandez-Patier, R., Moreno-Grau, S., Negral, L., Minguillón, M.C., Monfort, E.,
40 Sanz, M.J., Palomo-Marín, R., Pinilla-Gil, E., Cuevas, E., de la Rosa, J., Sánchez de la
41 Campa, A. (2008). Spatial and temporal variations in airborne particulate matter
42 (PM10 and PM2.5) across Spain 1999–2005. *Atmospheric Environment*, 42(17), 3964-
43 3979. doi: <http://dx.doi.org/10.1016/j.atmosenv.2006.10.071>
- 44 Reche, C., Viana, M., Brines, M., Perez, N., Beddows, D., Alastuey, A., Querol, X. (2015).
45 Determinants of aerosol lung-deposited surface area variation in an urban
46 environment. [Research Support, Non-U S Gov't]. *Sci Total Environ*, 517, 38-47.
- 47 Sardar, S.B., Fine, P.M., Mayo, P.R., Sioutas, C. (2005). Size-Fractionated Measurements of
48 Ambient Ultrafine Particle Chemical Composition in Los Angeles Using the

- 1 NanoMOUDI. *Environmental Science & Technology*, 39(4), 932-944. doi:
2 10.1021/es049478j
- 3 Schaap, M., Spindler, G., Schulz, M., Acker, K., Maenhaut, W., Berner, A., Wieprecht, W.,
4 Streit, N., Müller, K., Brüggemann, E., Chi, X., Putaud, J.P., Hitzemberger, R.,
5 Puxbaum, H., Baltensperger, U., ten Brink, H. (2004). Artefacts in the sampling of
6 nitrate studied in the "INTERCOMP" campaigns of EUROTRAC-AEROSOL. *Atmos.*
7 *Environ.*, 38(38), 6487-6496. doi: <http://dx.doi.org/10.1016/j.atmosenv.2004.08.026>
- 8 Schwarz, J., Štefancová, L., Maenhaut, W., Smolík, J., Ždímal, V. (2012). Mass and
9 chemically speciated size distribution of Prague aerosol using an aerosol dryer--the
10 influence of air mass origin. *Sci Total Environ*, 437, 348-362. doi:
11 10.1016/j.scitotenv.2012.07.050
- 12 Seinfeld, J.H., Pandis, S.N. (2006). Atmospheric Chemistry and Physics: From Air Pollution
13 to Climate Change, 2nd edition. *J. Wiley, New York*.
- 14 Sioutas, C. (2004). Development of New Generation Personal Monitors for Fine Particulate
15 Matter (PM) and its Metal Content. *NUATRC Research Report No. 2*.
- 16 Smolík, J., Dohányosová, P., Schwarz, J., Ždímal, V., Lazaridis, M. (2008). Characterization
17 of Indoor and Outdoor Aerosols in a Suburban Area of Prague. *Water Air Soil Pollut:*
18 *Focus*, 8(1), 35-47. doi: 10.1007/s11267-007-9141-y
- 19 Štefancová, L., Schwarz, J., Maenhaut, W., Chi, X., Smolík, J. (2010). Hygroscopic growth of
20 atmospheric aerosol sampled in Prague 2008 using humidity controlled inlets.
21 *Atmospheric Research*, 98(2-4), 237-248. doi:
22 <http://dx.doi.org/10.1016/j.atmosres.2010.04.009>
- 23 Štefancová, L., Schwarz, J., Mäkelä, T., Hillamo, R., Smolík, J. (2011). Comprehensive
24 Characterization of Original 10-Stage and 7-Stage Modified Berner Type Impactors.
25 *Aerosol Science and Technology*, 45(1), 88-100. doi: 10.1080/02786826.2010.524266
- 26 Stelson, A.W., Seinfeld, J.H. (1982). Relative humidity and temperature dependence of the
27 ammonium nitrate dissociation constant. *Atmospheric Environment (1967)*, 16(5),
28 983-992. doi: [http://dx.doi.org/10.1016/0004-6981\(82\)90184-6](http://dx.doi.org/10.1016/0004-6981(82)90184-6)
- 29 Talbot, N., Kubelova, L., Makes, O., Cusack, M., Ondracek, J., Vodička, P., Schwarz, J.,
30 Ždímal, V. (2016). Outdoor and indoor aerosol size, number, mass and compositional
31 dynamics at an urban background site during warm season. *Atmospheric Environment*,
32 131, 171-184. doi: <http://dx.doi.org/10.1016/j.atmosenv.2016.01.055>
- 33 Tursic, J., Grgic, I., Berner, A., Skantar, J., Cuhalev, I. (2008). Measurements of size-
34 segregated emission particles by a sampling system based on the cascade impactor.
35 [Research Support, Non-U S Gov't]. *Environ Sci Technol*, 42(3), 878-883.
- 36 Vodička, P., Schwarz, J., Ždímal, V. (2013). Analysis of one year's OC/EC data at a Prague
37 suburban site with 2-h time resolution. *Atmospheric Environment*, 77, 865-872. doi:
38 <http://dx.doi.org/10.1016/j.atmosenv.2013.06.013>
- 39 Wall, S.M., John, W., Ondo, J.L. (1988). Measurement of aerosol size distributions for nitrate
40 and major ionic species. *Atmospheric Environment (1967)*, 22(8), 1649-1656. doi:
41 [http://dx.doi.org/10.1016/0004-6981\(88\)90392-7](http://dx.doi.org/10.1016/0004-6981(88)90392-7)
- 42 Wang, H.-C., John, W. (1988). Characteristics of the Berner Impactor for Sampling Inorganic
43 Ions. *Aerosol Science and Technology*, 8(2), 157-172. doi:
44 10.1080/02786828808959179
- 45
46
47
48

1
2

3 Supplementary information



4

5 *Figure S1. Sampling location in Prague and impactors deployed in outdoor (top right) and*
6 *indoor environment (bottom right) (IPR, 2015).*



1

2 *Figure S2. Sampling location in Barcelona (BcnMap, 2015).*

2

3 *Table S1. Design parameters of the stages from nano-BLPI.*

3

Stage number	Lower cut sizes (μm)	Number of nozzles	Nozzle Diameter (mm)
9	1.95	1	3.60
8	1.00	39	0.70
7	0.49	17	0.60
6	0.24	8	0.54
5	0.095	43	0.27
4	0.062	88	0.25
3	0.039	142	0.25
2	0.024	237	0.25
1	0.011	408	0.25

4

5 *Table S2. Average mass concentrations for different ionic species during winter in outdoor*
 6 *and indoor air in Prague.*

5

6

Type of environment	Impactor	Mass ionic species ($\mu\text{g m}^{-3}$)							
		NO_3^-	SO_4^{2-}	NH_4^+	Cl^-	Na^+	K^+	Mg^{2+}	Ca^{2+}
Outdoor	BLPI (PM_{14})	6.72	5.72	3.78	0.40	0.22	0.20	0.03	0.14
	nano-BLPI ($\text{PM}_{1.95}$)	5.78	4.99	3.31	0.18	0.06	0.16	0.01	0.03
	nano-Moudi (PM_{10})	1.71	5.12	2.06	0.19	0.25	0.20	0.01	0.06
Indoor	BLPI (PM_{14})	0.49	2.15	0.78	0.05	0.10	0.10	0.01	0.05

nano-BLPI (PM _{1.95})	0.35	1.93	0.73	0.02	0.05	0.09	0.00	0.02
nano-Moudi (PM ₁₀)	0.34	1.53	0.53	0.03	0.13	0.08	0.00	0.05
Blank uncertainty*	1.3x10 ⁻³	9.4x10 ⁻⁴	2.0x10 ⁻⁴	3.0x10 ⁻⁴	2.0x10 ⁻⁴	2.0x10 ⁻⁴	1.0x10 ⁻⁴	3.0x10 ⁻⁴

1 * Recalculated per 1m³ of air for BLPI for 72 h sampling.