

Responses to Reviewer #1 – “Online molecular characterisation of organic aerosols in an atmospheric chamber using Extractive Electrospray Ionisation Mass Spectrometry” by P.J. Gallimore et al.

Reviewer comments are in blue text, author responses are in black text.

This is an interesting manuscript describing the efficacy of extractive electrospray ionization mass spectrometry (EESI-MS) as an online measurement technique for atmospheric chamber studies. They have used multiple online (EESI-MS and PTR-MS) and offline (ESI-MS) techniques to study the oxidation of α -pinene in the CASC chamber. They have shown that EESI-MS can be used to study SOA formed during chamber studies in almost real time (7-minute time resolution). The fact that EESI-MS is a soft ionization technique, it makes it more advantageous over the regular offline ESI-MS studies for chamber studies. They also compared MCM model results to EESI-MS and PTR-MS results, which showed very good correlations; it shows the potential of EESI-MS as an online measurement tool for chamber studies.

We thank the reviewer for the positive appraisal of the manuscript and respond point-by-point to the comments below.

General Comments - Introduction lacks the details of other online measurement techniques (like AMS, and DART-MS) used for α -pinene oxidation products, their findings and its comparison to EESI-MS.

We have added some references which use AMS for alpha-pinene SOA (page 2 lines 15-17): “A great deal of insight into SOA formation and aging from monoterpenes has been provided by established instruments such as the Aerosol Mass Spectrometer (Aiken et al., 2008; Chhabra et al., 2010; Shilling et al., 2009).”

We could not find specific uses of DART-MS for alpha-pinene SOA but have added references to Nah et al., (2013) and Zhao et al., (2017) as examples of the useful general insight provided by the technique (page 2 lines 30-31).

- More details about MCM model should be given in the SI in terms of reactions involved in the mechanism. So other laboratory trying to duplicate the work can do so easily.

We have included an additional section in the Supplement (page 4):

“Reaction scheme for MCM simulations

The reaction scheme for the degradation of α -pinene is based on the mechanism described in Saunders et al., (2003). All reactions involving the ozone-initiated oxidation of α -pinene and its products, including decomposition of reaction intermediates and secondary OH-mediated chemistry, were extracted from the MCM website (<http://mcm.leeds.ac.uk/MCM>) in June 2017. This mechanism extract comprises 313 explicit species.

We also included an auxiliary reaction to approximate the gradual introduction of ozone into the chamber (reaction S2):



Pre-O₃ does not participate in any other reactions, and is converted into O₃ on a timescale $\tau_{\text{pre}} = 1/k_{\text{pre}} = 3\text{-}30$ minutes, adjusted to reflect the experimental timescale for ozone introduction for each experiment.

The simulations were initialised with all species concentrations set to zero, apart from: α -pinene (MCM name APINENE), which was set to 45, 100 and 500 ppb for the low, medium and high concentration experiments respectively, and pre-O₃ (PREO3) which was adjusted to simulate the observed $[\text{O}_3]_{\text{max}}$ in each experiment (Table 1).”

- All the figures on Oxidation states of carbon against carbon number must include legends what size of the marker represents what intensity. They also should add the correct marker sizes in the inset of each figure, and if that is difficult, it should be included in SI then.

We have adapted Figures 3 and 4 to include a scale relating intensity to marker size, using a binned intensity scale for simplicity. This now also includes the inset regions. The figure captions have been updated accordingly (page 15 lines 3-5 and page 21 lines 1-3).

- EESI-MS studies of organic-inorganic particles: why was the study not performed on a compound that is more relevant to this study, for example, pinic acid?

We have added the following discussion (page 10, lines 25-28): “Tartaric acid is a highly oxygenated compound which is a relevant proxy for species present in aged organic aerosols. Its high water solubility and negligible volatility allow mixed TA-AS particles with precisely known composition to be prepared from solution.”

As noted on page 11 line 7, The use of TA also enables direct comparison with previous quantification work performed in Gallimore and Kalberer (2013).

- Although acids have higher sensitivity in negative ion mode, the inorganic salt has NH₄⁺ ions in them, thus positive ion mode would show [M+H]⁺ and [M+NH₄]⁺ ions for tartaric acid. Assuming all other parameters constant, the ratio of [M+H]⁺ to [M+NH₄]⁺ should match the mole fraction of the tartaric acid and ammonium sulfate in the atomized solvent. This would be much better way of quantitation than just looking at the acid signal in negative ion mode. I would strongly suggest repeating this particular experiment in positive ion mode.

We thank the reviewer for this thoughtful suggestion. However, we feel that quantification in positive ion mode is out of the scope of the current paper given that the subsequent emphasis on quantification uses negative ion mode (online/offline comparison, time series analysis). Instead, it would be better suited to an entire additional study.

It is not clear to us that $[\text{M}+\text{H}]^+ / [\text{M}+\text{NH}_4]^+$ would necessarily scale in a simple manner. This will depend on competitive ionisation processes – the relative affinities of the analyte for H⁺ and NH₄⁺, competition from contaminant Na⁺, and the absolute number of ions in the primary spray. We suspect the latter is far in excess of the number of analyte molecules extracted given that the relative quantification presented in Figure 2

and in Gallimore and Kalberer (2013) does not appear to “saturate” at higher mass loadings.

We have added a sentence to emphasise the purpose of section 3.1 (page 10 lines 21-23): “Specifically, we establish the potential impact of inorganic seed particles on the relative quantification of organic acids (detected as $[M-H]^-$) in the chamber experiments which follow.”

Specific comment: Page 1, line 30 Low visibility can also be added as an impact.

We now mention this as an impact (page 2 line 3).

Page 2 Line 13, The line is talking about soft-ionization in general, however, the reference (Zahardis et al) is not appropriate here. The reference does talk about soft ionization techniques, but the paper is a review of soft ionization techniques for AMS instrument specifically. AMS is mostly used for online studies and not off line measurements. Since the sentence for this reference is used for very generic off-line soft ionization MS techniques, the reference is not valid here.

We have replaced the Zahardis et al. reference with Hoffmann et al., (2011) (page 2 line 19), which features a discussion of soft ionisation MS techniques in the wider context of organic aerosol analysis.

Page 2 Line 17 Once again the paragraph is talking about general ESI-MS utility in atmospheric studies. The time resolution for ESI-MS is not hours, not for all kind of studies. However, it will be hours for chamber studies, if authors are refereeing to retention times of hours with respect to chamber studies it should be specified.

We have added clarification to our previous comments about time resolution (page 2 lines 23-25): “...the time resolution of measurements depends on the frequency at which aerosol samples are collected, which is typically an hour or more for chamber and ambient sampling.”

Page 3 line 1 Gallimore reference should be 2017a Also, this particular reference is not published yet, thus the conclusion of this study cannot be used as the basis of claiming that EESI-MS can be used for relative quantitation.

The reference has now been published; the full citation is given in the References section and is referred to as Gallimore et al., (2017a) in the text (page 3, line 10), consistent with the rest of the manuscript.

Page 4 Line 22 Authors can probably use particle size distributions of Tartaric acid (TA) and Ammonium Sulfate particles to confirm that they are truly internally mixed. If these particles are not internally mixed they probably will show a bimodal distribution. It should be checked for all mole fractions studied, it is possible that higher concentration of ammonium sulfate will lead to a bimodal distribution.

Thank you for this insight. We have added (page 4, lines 27-28): “A single mode was observed in the particle size distribution for all nebuliser solutions; particles were therefore assumed to be internally mixed...”

Page 6 Line 10 Was the ESI solvent prepared 1:1 by volume or by weight. Solvent flow rate should also be provided.

We now mention (page 6, line 21): “...a water-methanol 1:1 mixture by volume...” and state (page 6, lines 23-24): “The solvent flow rate was set to 10 $\mu\text{L min}^{-1}$.”

Page 6 line 13-14 Authors just described ESI solvent and voltage details previous to these lines. Thus it is really ESI description, not an EESI-MS description. I would suggest adding line 16-19 that describes the particle flow rate to solvent spray before line 13-14.

We have moved the particle flow discussion above the first mention of EESI(+) and EESI(-) operating conditions (page 6, line 26).

Figure 1 Should show the position of three-way valve.

Figure 1 has been updated accordingly (page 7), and also now includes the optional HEPA filter discussed in response to Reviewer 2.

Page 7 line 6-8 These lines are confusing. Do the authors mean the following? “Air was then pushed through the reservoir and into the EESI source at 1 L min⁻¹ and a sample spectrum was acquired.” If yes, it should be corrected. If No, more clarification of the set-up is required.

We have corrected “flow tube” to “reservoir” as suggested (page 7 line 14).

Page 7 line 23 Was formic acid added to the final extract before nano-ESI? If so, details should be added.

We now mention (page 8, lines 5-6): “...and 0.1 % by volume formic acid was added to the extract”

Page 7 line 25 Is 1.4kV potential difference correct? Because for EESI it is 3kV. Why the difference for the same solvent configuration.

This potential difference is correct. The lower solvent flow rates used in nanoESI are commonly paired with lower potential differences compared to conventional ESI. We have not updated the text.

Page 9 line 1 Reference and explanation should be provided for the rate constant assumption.

We have added the following sentence (page 9, lines 24-26): “Exothermic proton transfer reactions occur at a rate close to the collision limit (Blake et al., 2009) and known rate constants for a variety of VOCs are within 50 % of this value (Smith and Spanel, 2005).”

Page 9 line 18 References should be provided for which previous studies were used to identify the major aerosol composition.

We now refer to “previous studies referenced in Table 2” (page 10 lines 12-13) which provides a summary of major products considered in this manuscript.

Page 10 figure 1 Y axis should be adjusted to show the complete error bar of the first purple triangle marker at a mole fraction of 0.5. Why that particular point has so much error should be explained in the text as well.

The y-axis of Figure 2 has now been rescaled accordingly (page 11). The absolute error on this marker is low, but, following background subtraction, appears large because the data are presented on a log scale. We have not changed the text.

Table 2 Once again why wasn't $[M+NH_4]^+$ seen in positive ion mode?

We have added the following discussion (page 8, lines 20-29): “This removes formulae which fall outside a 2 ppm mass tolerance and those deemed implausible based on their atomic ratios. By strictly limiting permitted elements, we reduce the number of erroneous permutations of formulae that coincide with the measured m/z . Based on the oxygenated VOCs expected for α -pinene SOA (Table 2), we retained assignments containing only carbon, hydrogen and oxygen, and permitted sodium adduct formation in positive ion mode. Nitrogen-containing compounds are not expected to form via ozonolysis, but we note that this treatment excludes possible $[M + NH_4]^+$ adducts derived from the ammonium sulfate seed particles. However, in the raw data, such clusters were not apparent for major positive mode species such as pinonaldehyde.”

As discussed above in reply to general comment #5, we speculate that this is a consequence of the apparent large excess of primary electrospray ions (favouring H^+ and Na^+) relative to organic and ammonium analytes.

Page 13 line 1 The presence of $[M+H-H_2O]^+$ peak in Doezema et al studies can be explained in many ways, different instrument parameters for the two studies, different inlet, and mass analyzer voltages etc. Higher capillary Voltage used in that study could simply be due to the combination of solvent composition, solvent flow rate and capillary diameter required to get a good Taylor cone. Authors can only compare the capillary voltage if all other parameters are equal.

We agree that the other parameters mentioned by the reviewer may also be important and have deleted the specific reference to voltage. The revised sentence now reads (page 14, lines 1-3): “This suggests that the choice of EESI parameters may be an important determinant of fragmentation.”

Page 16 I would suggest moving figure S5 to the main text.

We have included this as Figure 5 in the main text (page 17) and deleted it from the Supplement. Later figures have been renamed accordingly.

Page 16 line 14-16 If more oxidized species are present in the particle than it could possibly suggest that EESI-MS solvent is extracting some surface of the particle only rather than the entire particle as assumed in Gallimore et al 2013 and I am assuming for this study too. Many studies on oxidation of monoterpenes (Zhao et al 2016 ACP, 16, 3245; Davis et al 2015,

Chem.Sci. 6, 7020; Zhao et al 2017, *AMT*, 10, 1373 ; Trostl et al *Nature* 2016, 533, 527–531) have suggested that low molecular weight compounds with high Oxidation state are present in the core of the particle and are responsible for new particle formation. Whereas, low molecular weight compounds with low Oxidation state are responsible for the growth of the particle and are usually present on the surface of the particle. Thus the lack of peaks at high m/z in EESI-MS (Figure S5) suggests that the solvent is extracting the surface of the particle only or at least not the entire particle. Collected particles on the filter analyzed by ESI-MS show many peaks at higher m/z , suggesting ESI is able to sample entire particle, which is expected. But, if the presence of peaks at higher m/z in ESI-MS is due to oligomers (eg $2M+H$ of pinonaldehyde) then it should be confirmed using MS/MS studies. Identifying the source of these higher m/z peaks in ESI-MS is important to identifying and understand EESI-MS extraction efficiency.

It has been shown that other MS techniques such as Direct Analysis in Real Time (DART) only analyse an outer portion of particles (Nah et al., 2013). However, our tests on EESI-MS, both here (Figure 2) and previously in Gallimore and Kalberer (2013), show the MS signal scales with total particle mass, independent of particle size for the range tested. While the EESI ionisation process is not yet fully understood (Law et al., 2010), we believe aerosol components in the core of particles are at least available for extraction and ionisation under these conditions. Further work is required to establish at what particle size and/or total mass this linearity may break down.

Higher m/z ions were identified using both ESI-MS and EESI-MS analyses here (see Figure 4 and the new Figure 5). Many have been positively identified as in-particle oligomers (rather than ionisation artefacts) in previous studies (e.g. (Kristensen et al., 2013)). As discussed (page 18, lines 1-3), our hypothesis is that the larger number seen in the offline analysis is a concentration/sensitivity effect. We should also point out that offline ESI-MS is known to suffer from positive and negative sampling artefacts, and competitive ionisation effects. It therefore does not necessarily provide a definitive point of comparison for the true “bulk” composition.

We have added an additional sentence (page 18, lines 9-11): “Horan et al., (2012) found that the relative abundance of oligomers was also higher in filter samples than their online AESI method, which was attributed to a negative filter sampling artefact – evaporation of semi-volatile material (predominantly monomers) during collection.”

References

Aiken, A. C., Decarlo, P. F., Kroll, J. H., Worsnop, D. R., Huffman, J. A., Docherty, K. S., Ulbrich, I. M., Mohr, C., Kimmel, J. R., Sueper, D., Sun, Y., Zhang, Q., Trimborn, A., Northway, M. J., Ziemann, P. J., Canagaratna, M. R., Onasch, T. B., Alfarra, M. R., Prevot, A. S. H., Dommen, J., Duplissy, J., Metzger, A., Baltensperger, U. and Jimenez, J. L.: O / C and OM / OC Ratios of Primary , Secondary , and Ambient Organic Aerosols with High-Resolution Time-of-Flight Aerosol Mass Spectrometry, *Environ. Sci. Technol*, 42(12), 4478–4485, 2008.

Blake, R. S., Monks, P. S. and Ellis, A. M.: Proton-transfer reaction mass

- spectrometry., *Chem. Rev.*, 109(3), 861–96, doi:10.1021/cr800364q, 2009.
- Chhabra, P. S., Flagan, R. C. and Seinfeld, J. H.: Elemental analysis of chamber organic aerosol using an aerodyne high-resolution aerosol mass spectrometer, *Atmos. Chem. Phys.*, 10, 4111–4131, doi:10.5194/acp-10-4111-2010, 2010.
- Gallimore, P. J. and Kalberer, M.: Characterizing an extractive electrospray ionization (EESI) source for the online mass spectrometry analysis of organic aerosols, *Environ. Sci. Technol.*, 47(13), 7324–31, doi:10.1021/es305199h, 2013.
- Gallimore, P. J., Griffiths, P. T., Pope, F. D., Reid, J. P. and Kalberer, M.: Comprehensive modeling study of ozonolysis of oleic acid aerosol based on real-time, online measurements of aerosol composition, *J. Geophys. Res. Atmos.*, 122, 4364–4377, doi:10.1002/2016JD026221, 2017a.
- Hoffmann, T., Huang, R.-J. and Kalberer, M.: Atmospheric Analytical Chemistry, *Anal. Chem.*, 83(12), 4649–64, doi:10.1021/ac2010718, 2011.
- Horan, A. J., Gao, Y., Hall, W. A. and Johnston, M. V: Online Characterization of Particles and Gases with an Ambient Electrospray Ionization Source, *Anal. Chem.*, 84, 9253–9258, 2012.
- Kristensen, K., Enggrob, K. L., King, S. M., Worton, D. R., Platt, S. M., Mortensen, R., Rosenoern, T., Surratt, J. D., Bilde, M., Goldstein, A. H. and Glasius, M.: Formation and occurrence of dimer esters of pinene oxidation products in atmospheric aerosols, *Atmos. Chem. Phys.*, 13(7), 3763–3776, doi:10.5194/acp-13-3763-2013, 2013.
- Law, W. S., Wang, R., Hu, B., Berchtold, C., Meier, L., Chen, H. and Zenobi, R.: On the mechanism of extractive electrospray ionization., *Anal. Chem.*, 82(11), 4494–500, doi:10.1021/ac100390t, 2010.
- Nah, T., Chan, M., Leone, S. R. and Wilson, K. R.: Real Time in Situ Chemical Characterization of Submicrometer Organic Particles Using Direct Analysis in Real Time-Mass Spectrometry, *Anal. Chem.*, 85, 2087–95, doi:10.1021/ac302560c, 2013.
- Saunders, S. M., Jenkin, M. E., Derwent, R. G. and Pilling, M. J.: Protocol for the development of the Master Chemical Mechanism, MCM v3 (Part A): tropospheric degradation of non-aromatic volatile organic compounds, *Atmos. Chem. Phys.*, 3, 161–180, 2003.
- Shilling, J. E., Chen, Q., King, S. M., Rosenoern, T., Kroll, J. H., Worsnop, D. R., DeCarlo, P. F., Aiken, a. C., Sueper, D., Jimenez, J. L. and Martin, S. T.: Loading-dependent elemental composition of α -pinene SOA particles, *Atmos. Chem. Phys.*, 9, 771–782, doi:10.5194/acp-9-771-2009, 2009.
- Smith, D. and Spangel, P.: SELECTED ION FLOW TUBE MASS SPECTROMETRY (SIFT-MS) FOR ON-LINE TRACE GAS ANALYSIS, *Mass Spectrom. Rev.*, 661–700, doi:10.1002/mas.20033, 2005.
- Zhao, Y., Fairhurst, M. C., Wingen, L. M., Perraud, V. and Ezell, M. J.: New insights into atmospherically relevant reaction systems using direct analysis in real-time mass spectrometry (DART-MS), , 1373–1386, doi:10.5194/amt-10-1373-2017, 2017.

Responses to Reviewer #2 – “Online molecular characterisation of organic aerosols in an atmospheric chamber using Extractive Electrospray Ionisation Mass Spectrometry” by P.J. Gallimore et al.

Reviewer comments are in blue text, author responses are in black text.

This manuscript (acp-2017-656) reports the application of extractive electrospray ionisation mass spectrometry (EESI-MS) to the analysis of chamber aerosol produced by reaction of the monoterpene α -pinene with O₃. Gas phase reactants and products were monitored with proton transfer reaction mass spectrometry (PTR-MS), whereas particle phase products were monitored with EESI-MS with time resolution on the order of 7 min. The time dependence of the MS signals for α -pinene (by PTR-MS) and pinonic acid, pinic acid, and OH-pinonic acid (by EESI-MS) correlated well with predictions from the Master Chemical Mechanism (MCM). The signal intensity of reaction products correlated approximately linearly in log-log space with MCM predictions. Additionally, EESI-MS of test particles containing tartaric acid and ammonium sulfate in known relative molar ratios resulted in a linear signal with increasing mass concentration across all organic-inorganic molar ratios down to 1:1.

This manuscript is well written and the experiments appear to be carefully performed. The figures are well constructed and easy to interpret. This manuscript is within the scope of Atmospheric Chemistry and Physics and will be suitable for publication once the comments below are satisfactorily addressed.

We thank the reviewer for the positive appraisal of the manuscript and respond to the comments below.

Comments:

1. One area where this manuscript could be significantly strengthened is in clarifying how much of the EESI-MS signal may arise from gas phase molecules. The chamber contains both organic particles and semivolatile compounds that are going to be present in both the gas phase and the particle phase. It appears the authors use a charcoal denuder to remove the gas phase before sampling into the EESI-MS. However, the authors provide no figure or discussion that quantifies how much, if any, of the EESI-MS signal may arise from gas phase products. The authors should discuss this in the revised manuscript. Resolving whether signal arises from gas or particle could be easily tested by placing a filter to remove the particles before the EESI-MS inlet and monitoring the resulting signal. Note that even if the charcoal denuder removes much of the gas phase, it is possible that compounds that were in the particle phase may partition back to the gas phase during the residence time in the 10 L reservoir. This is an important point, as the authors are comparing their EESI-MS results, which are assumed to be entirely particle phase, to MCM predictions, which is a gas phase model.

We agree that this is an insightful additional test and followed the reviewer’s suggestion of performing additional experiments using a filter. The manuscript has been modified in the following places:

Page 7, lines 15-17: “An optional High Efficiency Particle Air (HEPA) filter (HEPA CAP, Whatman) was used to test the possible contribution of gas phase species to the observed MS signal.”

Page 19 line 24-page 20 line 15: “The semi-volatile nature of SOA means that both gas- and particle-phase species will be present in the chamber. We examined whether gas-phase species contribute to our observed EESI(-)-MS signal under the “medium” reaction conditions by removing particles from the sample flow using a HEPA filter (Figure 1). With particles filtered out, none of the species listed in Table 2 could be detected above levels observed for the solvent blanks. This was also the case even if the charcoal denuder in Figure 1, intended to remove gas-phase species, was bypassed.

The aerosol mass loading in the chamber ($\sim 300 \mu\text{g m}^{-3}$) would strongly bias most of the compounds in Table 2 towards the particle phase. For instance, the most abundant ion, pinic acid, has a vapour pressure $\sim 2 \mu\text{g m}^{-3}$ at 294 K (Bilde and Pandis, 2001), so $> 99\%$ would be expected to reside in the particle phase based on an absorptive partitioning argument (Pankow, 1994). This might explain the lack of detected species in the present SOA system. However, a number of studies have detected gas-phase species using an electrospray source, e.g. (Horan et al., 2012; Wu et al., 2000; Zhao et al., 2017). The ion source design and operating parameters appear important in determining the ionisation efficiency and mechanism (uptake into droplets or gas-phase chemical ionisation). Future work to simultaneously detect semi-volatile species in both phases, and understand the relative efficiencies of gas- and particle-phase ionisation, is therefore merited.”

Abstract (page 1, lines 19-20): “Under our experimental conditions, EESI-MS signals arise only from particle-phase analytes.”

Conclusions (page 26, line 25-27): “Our limited tests with this EESI-MS configuration show that the signal arising is a result of droplet-particle collisions, with negligible contribution from gas-phase analytes.”

2. When the authors examine relative quantification in the mixed organic-inorganic system, they observe that down to a 1:1 organic:inorganic mole fraction the MS signal intensity scales linearly with organic aerosol mass concentration (Fig. 2). The authors also suggest (page 10, line 20) that suppression of signal may be occurring, but that it is small. It is unclear why the authors did not continue this experiment to higher inorganic aerosol (lower organic aerosol) mole fractions to confirm this suggestion. More discussion is required on this point.

We have added the following discussion to emphasise the purpose of Figure 2 (page 10, lines 21-23): “Specifically, we establish the potential impact of inorganic seed particles on the relative quantification of organic acids (detected as $[\text{M}-\text{H}]^-$) in the chamber experiments which follow.” $5 \mu\text{g m}^{-3}$ ammonium sulfate seed particles were added to the chamber, and this corresponded to small fractions of the aerosol mass during MS analysis. These conditions are covered by Figure 2.

We agree that considering a wider parameter space (including particle composition) in future is desirable to extend the applicability, and understand potential limitations of, the EESI-MS technique.

3. The authors should include in the revised manuscript the values for the low mass cut-offs on their mass analysers. As illustrated in Fig. S4 and visualised in Fig. 3, the EESI-MS and PTR-MS spectra appear very different. However, it is not entirely clear if this is due wholly to the different compositions in the gas and particle phase or due to the mass ranges that can be studied with each instrument. The PTR-MS spectrum contains a large number of ions below 100 m/z whereas the EESI-MS spectra do not, but it is not clear in the discussion whether the Orbitrap would necessarily be able to analyse effectively below 100 m/z.

The mass ranges for the mass analysers are already stated in the methods section (page 8, line 12: m/z 100-500 for EESI-MS; page 9 line 9: m/z 10-500 for PTR-MS). We have added the following emphasis in the discussion (page 12, lines 14-15): “The low mass thresholds of the EESI-MS and PTR-MS mass analysers were m/z 100 and 10 respectively in this study.”

References

- Bilde, M. and Pandis, S. N.: Evaporation Rates and Vapor Pressures of Individual Aerosol Species Formed in the Atmospheric Oxidation of alpha- and beta-Pinene, *Environ. Sci. Technol.*, 35(16), 3344–3349, 2001.
- Horan, A. J., Gao, Y., Hall, W. A. and Johnston, M. V.: Online Characterization of Particles and Gases with an Ambient Electrospray Ionization Source, *Anal. Chem.*, 84, 9253–9258, 2012.
- Pankow, J. F.: An absorption model of the gas/aerosol partitioning involved in the formation of secondary organic aerosol, *Atmos. Environ.*, 28(2), 189–193, 1994.
- Wu, C., Siems, W. F. and Hill Jr., H. H.: Secondary Electrospray Ionization Ion Mobility Spectrometry / Mass Spectrometry of Illicit Drugs, *Anal. Chem.*, 72(2), 396–403, 2000.
- Zhao, Y., Chan, J. K., Lopez-Hilfiker, F. D., McKeown, M. A., Ambro, E. L. D., Slowik, J. G., Riffell, J. A. and Thornton, J. A.: An electrospray chemical ionization source for real-time measurement of atmospheric organic and inorganic vapors, *Atmos. Meas. Tech.*, 3609–3625, 2017.

Online molecular characterisation of organic aerosols in an atmospheric chamber using Extractive Electrospray Ionisation Mass Spectrometry

5 Peter J. Gallimore¹, Chiara Giorio^{1,2}, Brendan M. Mahon¹ and Markus Kalberer¹

¹ Department of Chemistry, University of Cambridge, Lensfield Road, Cambridge, CB2 1EW, UK.
² now at Aix Marseille Univ, CNRS, LCE Marseille, France.

Correspondence to: Markus Kalberer (markus.kalberer@atm.ch.cam.ac.uk)

Abstract. The oxidation of biogenic volatile organic compounds (VOCs) represents a substantial source of secondary organic aerosol (SOA) in the atmosphere. In this study, we present online measurements of the molecular constituents formed in the gas and aerosol phases during α -pinene oxidation in the Cambridge Atmospheric Simulation Chamber (CASC). We focus on characterising the performance of Extractive Electrospray Ionisation (EESI) mass spectrometry (MS) for particle analysis. A number of new aspects of EESI-MS performance are considered here. We show that relative quantification of organic analytes can be achieved in mixed organic-inorganic particles. A comprehensive assignment of mass spectra for α -pinene derived SOA in both positive and negative ion modes is obtained using an ultra-high resolution mass spectrometer. We compare these online spectra to conventional offline ESI-MS and find good agreement in terms of the compounds identified, without the need for complex sample work-up procedures. Under our experimental conditions, EESI-MS signals arise only from particle-phase analytes. High time resolution (7 minutes) EESI-MS spectra are compared with simulations from the near explicit Master Chemical Mechanism (MCM) for a range of reaction conditions. We show that MS intensities scale with modelled concentrations for condensable products (pinonic acid, pinic acid, OH-pinonic acid). Relative quantification is achieved throughout SOA formation as the composition, size and mass (5-25 2400 $\mu\text{g m}^{-3}$) of particles is evolving. This work provides a robust demonstration of the advantages of EESI-MS for chamber studies over offline ESI-MS (time resolution, relative quantification) and over “hard” online techniques (molecular information).

1 Introduction

Airborne particulate matter has significant impacts on global climate (Hallquist et al., 2009), ~~and~~ human health (Dominici et al., 2006) and visibility (Husar et al., 1981). Organic compounds typically comprise around 50% of submicron aerosol mass (Jimenez et al., 2009). Most of this is secondary and biogenic in origin (Hallquist et al., 2009); the oxidation of biogenic volatile organic compounds (VOCs) such as monoterpenes and isoprene represents a major source of atmospheric secondary organic aerosol (SOA) (Kroll and Seinfeld, 2008; Ziemann and Atkinson, 2012). However, SOA formation processes remain highly uncertain and this is regarded as a major weakness in the current understanding and model representation of atmospheric aerosols (Boucher et al., 2013). The chemistry involved is complex, and the range of organic compounds present in the atmosphere is extremely diverse (Goldstein and Galbally, 2007). Understanding how SOA components form and react is therefore a conceptual and analytical challenge (Noziere et al., 2015).

Identifying and quantifying individual organic components in this complex mixture is commonly achieved using mass spectrometry (MS). A great deal of insight into SOA formation and aging from monoterpenes has been provided by established instruments such as the Aerosol Mass Spectrometer (Aiken et al., 2008; Chhabra et al., 2010; Shilling et al., 2009). Of particular utility for understanding organic reaction mechanisms are so-called “soft” ionisation techniques, which retain molecular structure during ion formation (~~Zahradis et al., 2011~~) (Hoffmann et al., 2011). Most conventional soft ionisation MS is “offline”, where chemical analysis is performed subsequent to sampling. Techniques such as electrospray ionisation (ESI) MS have yielded extensive insight into aerosol chemical processes (Claeys et al., 2009; Edney et al., 2005; Kampf et al., 2012; Kourtchev et al., 2014). However, there are drawbacks to offline ESI-MS: the time resolution of measurements depends on the frequency at which new aerosol samples are collected, which is typically an hour or more for chamber and ambient sampling, limited time resolution of typically an hour or more; the There is also potential for sampling artefacts (Turpin et al., 2000), and a lack of analyte quantification when used in a direct-infusion mode.

A number of recent studies have therefore developed online or semi-continuous atmospheric-pressure ionisation (API) MS techniques (Bateman et al., 2010; Brüggemann et al., 2015; Clark et al., 2014; Nah et al., 2013; Pereira et al., 2014; Vogel et al., 2013; Zhang et al., 2015; Zhao et al., 2017b). In this paper, we focus on the application of one such approach to organic aerosol analysis, namely extractive electrospray ionisation (EESI) MS. The EESI process predominantly forms molecular ions ($[M + H]^+$ and $[M - H]^-$) and is able to efficiently ionise organic analytes even in

complex sample matrices such as urine (Devenport et al., 2014), beer (Zhu et al., 2010) and olive oil (Law et al., 2010). Doezema et al., (2012) demonstrated an initial application of EESI-MS to organic aerosols, identifying a number of products formed from α -pinene ozonolysis in positive ion mode. Horan et al., (2012) reported a related technique for particle and gas phase chemical characterisation, ambient electrospray ionisation (AESI).

Our earlier study reported the first quantification of the EESI aerosol extraction process for carboxylic acid particles (Gallimore and Kalberer, 2013). The detected MS intensity scaled in direct proportion with the aerosol mass concentration and was independent of particle diameter in the ranges studied (3-600 $\mu\text{g m}^{-3}$, 70-200 nm). Gallimore et al., (~~Gallimore et al., 2017a~~)(2017) applied the technique for the first time to characterising the kinetics of particle-phase reactions, using the ozonolysis of oleic acid particles as a model system. Changes in relative intensities of ions were used successfully as a proxy for relative concentrations and complex oligomeric species could be detected with minimal molecular fragmentation. Very recently, we demonstrated the ability of the ion source to stably operate for several hours during the evolution of limonene SOA (Gallimore et al., 2017b).

In the current study, we evaluate in detail the use of EESI-MS for atmospheric chamber experiments. Large-volume atmospheric chambers have proven to be a valuable means of exploring volatile organic compound (VOC) oxidation mechanisms because a simplified subset of reactions can be investigated under well-defined conditions (Cocker et al., 2001; Gallimore et al., 2017b; Paulsen et al., 2005). We investigate SOA formation from the ozone-initiated oxidation of α -pinene, the most abundant monoterpene in the troposphere (with estimated emissions $\sim 60 \text{ Tg yr}^{-1}$, Guenther et al., (2012)). α -pinene forms SOA from the condensation of low volatility oxidised products, and is a major source of biogenic aerosol (Claeys et al., 2009; Jenkin, 2004; Kristensen et al., 2013). Species identified here are compared to previous experimental studies and model representations of the oxidation pathways.

Ultra-high resolution mass spectra of α -pinene SOA are obtained using EESI operating in both ion polarities (+ and -). EESI-MS is used alongside Proton Transfer Reaction (PTR) MS (Blake et al., 2009) to obtain molecular-level gas and particle phase information with high time resolution. We are particularly interested in the ability of EESI-MS to provide quantitative information such as concentration changes during aerosol formation and aging. We initially confirm that relative quantification of individual organic species is still possible in mixed organic-inorganic particles. This is then extended to chemically complex chamber SOA, where the particle composition, size

and mass is evolving over time. In particular, we find that EESI(-) MS intensities of condensable products of α -pinene oxidation (pinonic acid, pinic acid, OH-pinonic acid) map quantitatively onto simulated concentrations from the Master Chemical Mechanism (Jenkin, 2004). These findings support the continued use of EESI-MS for chamber experiments and prompt further development of the technique to improve sensitivity for other applications.

2 Methods

2.1 Quantification of mixed organic-inorganic particles with EESI

An aerosol generation system, described in detail in Gallimore and Kalberer (2013) was used to produce model aerosols for quantifying the extraction and ionisation of organic compounds in the presence of inorganic salts (Figure S1).

Aerosols were produced from aqueous solutions using a custom made constant-output atomiser. Solutions containing L-tartaric acid (99 %, Aldrich) and ammonium sulfate (99.5 %, Fluka) in water (HPLC grade, Rathburn) were prepared. The total solute concentration was held constant at 0.1 mol L⁻¹ and four stock solutions were prepared with the following tartaric acid mole fractions (x_{TA}): 1, 0.98, 0.9, 0.5, the remainder being composed of ammonium sulfate ($x_{AS} = 1 - x_{TA}$). The nebuliser was supplied with N₂ (oxygen-free nitrogen, BOC) at a pressure of 3 bar to produce an output flow rate of 1.3 L min⁻¹.

A silica diffusion dryer was used to produce dry particles (<10 % RH). The dried polydisperse particles were size-selected in the range 50-200 nm prior to EESI-MS analysis using a differential mobility analyser (DMA) (TSI model 3081). The outflow from the DMA was split, with 0.3 L/min sampled by a condensation particle counter (CPC) (TSI model 3775) to measure the size-selected particle concentration. The remaining 1 L min⁻¹ was introduced into the EESI source. Particle mass concentrations were calculated from the CPC number concentration by assuming an aerosol density of 1.78 g cm⁻³, close to the bulk densities of tartaric acid (1.79 g cm⁻³) and ammonium sulfate (1.77 g cm⁻³). A single mode was observed in the particle size distribution for all nebuliser solutions: Particles were therefore assumed to be internally mixed with a composition representative of the bulk nebuliser solution. The mass concentrations were corrected for the transmission of multiply-charged particles through the DMA according to the method described in Gallimore and Kalberer (2013).

2.2 Atmospheric chamber operation

Experiments on the oxidation of biogenic VOCs were performed in the newly commissioned Cambridge Atmospheric Simulation Chamber (CASC) which is characterised in detail in Gallimore et al., (2017b). Aspects of the chamber operation relevant to the results in this paper are described briefly here (Figure S2).

The chamber consists of a 5.4 m³ Fluorinated Ethylene Propylene (FEP) bag housed in an aluminium frame. Gas introduction and sampling are achieved through stainless steel flanges containing Swagelok fittings at the front and rear of the chamber. A series of mass flow controllers (MKS, 5-200 L min⁻¹) are used to control flows into the chamber. The frame houses opaque perspex screens to block light from entering the chamber during “dark” reactions. The chamber is cleaned between experiments by flushing clean air from a zero air generator (Parker Hannifin KA-MT2) through the chamber using a mass flow controller and pump (Charles Austen ET200) at matched 200 L min⁻¹ flows. Ozone and “hard” UV lights may also optionally be used during cleaning.

Aerosol formation was investigated for the dark reaction between α -pinene and ozone in the presence of inorganic seed particles. The chamber was filled with clean air from the zero air generator. Water vapour was introduced by bubbling air at 5 L min⁻¹ through a heated round-bottomed flask containing water. The chamber’s relative humidity (RH) and temperature were monitored using a Honeywell HIH4000 probe and were typically 60% RH and 291 K respectively in these experiments. Seed aerosols were produced from ammonium sulfate solutions using a nebuliser and dryer as described above. The seed particle concentration in the chamber was $\sim 5 \mu\text{g m}^{-3}$. α -pinene (98 %, Aldrich) was evaporated into the chamber from an impinger using clean air. Ozone was produced by flowing air through a photolysis tube containing a mercury UV lamp (Appleton Woods) at 10 L min⁻¹, corresponding to a change in the chamber [O₃] of $\sim 50 \text{ ppb min}^{-1}$. The concentration in the chamber was monitored using a photometric ozone analyser (Thermo Scientific model 49i) and was introduced until [O₃]/[α -pinene]₀ ~ 3 was achieved (~ 3 -30 minutes). The range of α -pinene and ozone concentrations used in the chamber are detailed in Table 1.

Experiment	[α -pinene] ₀ (ppb)	[O ₃] _{max} (ppb)	Online MS sampling
Low	45	145	PTR, EESI(-)
Medium 1	99	320	PTR, EESI(-)
Medium 2	100*	325	EESI(+)
High	502	1450	PTR, EESI(-)

Table 1: Conditions used in the chamber experiments in this paper. In all cases, the chamber humidity was adjusted to 60% RH and $\sim 5 \mu\text{g m}^{-3}$ ammonium sulfate seed particles were introduced prior to α -pinene and ozone introduction. (*) Estimated concentration since PTR-MS not used in this experiment.

- 5 An air “sprinkler” system, consisting of a 2 m PTFE tube with a series of small holes along its length, was supplied with high pressure bursts of air to mix the chamber constituents without recourse to a fan. The air sprinkler leads to the addition of ~ 100 L clean air during ozone introduction, and results in a mixing time of a few minutes (Gallimore et al., 2017b). The size distribution of aerosols in the chamber was monitored using an SMPS (TSI model 3936). To enable presentation of data as measured, including “raw” EESI-MS time series, wall-loss correction was not attempted and therefore we focus primarily on the initial time following ozone introduction, where aerosol production will dominate over loss to the chamber walls.

2.3 EESI source operation and chamber sampling

- 15 The EESI source is described in detail in Gallimore and Kalberer (2013). Briefly, it consists of a custom-built aerosol injector and housing which is interfaced with a commercially-available electrospray ionisation (ESI) source. The primary solvent electrospray can generate droplets with positive or negative charges depending on the potential difference between the ESI probe and the mass spectrometer. Particle-droplet collisions dissolve the aerosol analytes, which are ionised and
20 ejected into the gas phase by a Coulomb explosion mechanism.

- Here the primary solvent was a water-methanol 1:1 mixture by volume (Optima LC grade solvents, Fisher Scientific) containing 0.05 % formic acid (90 %, Breckland) as a spray modifier. The solvent flow rate was set to $10 \mu\text{L min}^{-1}$. The nitrogen sheath gas flow rate was set to 0.8 L min^{-1} . The
25 potential difference was set to +3.0 and -3.0 kV for positive and negative ion modes respectively. The aerosol injector delivers particles into the primary solvent spray at a flow rate of 1 L min^{-1} . We refer to these operating conditions as EESI(+) and EESI(-) for the remainder of the manuscript.

- ~~The aerosol injector delivers particles into the primary solvent spray at a flow rate of 1 L min^{-1} .~~
30 ~~Particle droplet collisions dissolve the aerosol analytes, which are ionised and ejected into the gas phase by a Coulomb explosion mechanism.~~ The commercial ESI housing was found not to be air tight, so a batch sampling procedure was adopted to introduce particles from the chamber into the EESI source (Figure 1).

Formatted: Superscript

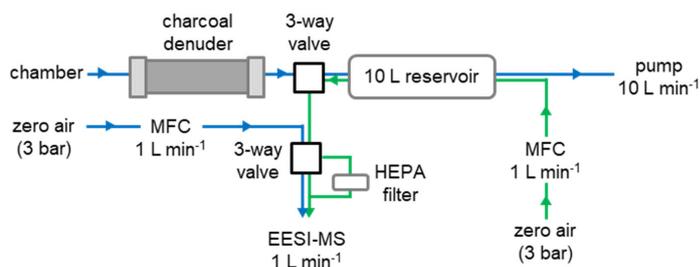


Figure 1: Batch sampling system used to supply the EESI source with chamber air in a two-step process. 1. (blue lines): air is drawn from the chamber into an intermediate 10 L reservoir, during which time the EESI source is flushed with zero air and a blank spectrum is acquired (3.5 minutes). 2. (green lines): chamber air from the flow tube is pushed through to the EESI source to acquire a sample spectrum (3.5 minutes).

Air was drawn from the chamber at 10 L min^{-1} through a charcoal denuder, used to remove ozone and VOCs, into an intermediate reservoir of approximately 10 L. During this time, the aerosol injector and EESI source were flushed with 1 L min^{-1} synthetic air (zero-grade, BOC) to obtain a “blank” mass spectrum and maintain a constant gas flow into the source (blue flow configuration in Figure 1). After 3.5 minutes, the air flush and pump were switched off and three-way valves were used to isolate the reservoir from the chamber and connect it to the EESI source. Air was then pushed through the flow tube reservoir and into the source at 1 L min^{-1} and a sample mass spectrum acquired (green flow configuration in Figure 1). An optional High Efficiency Particle Air (HEPA) filter (HEPA CAP, Whatman) was used to test the possible contribution of gas phase species to the observed MS signal.

Repetition of this cycle allowed batch sampling with a time resolution of 7 minutes. Particle losses using the sampling system in this way were characterised using an SMPS and were $\sim 10 \%$ of the total aerosol mass. Chamber air in the reservoir volume was not expected to be diluted significantly by the 1 L min^{-1} inflow during sample acquisition under the laminar flow conditions used (discussed in the Supplementary Information).

2.4 SOA filter sampling and analysis

Filter samples of SOA were collected during the same experiments as the online composition measurements. The sampling and analysis protocol was based on that described in Kourtchev et al.,

(2014). Briefly, particles were drawn through a charcoal denuder and collected onto cleaned quartz fibre filters (Pallflex® Tissuquartz 2500QAT-UP, 47 mm diameter) 1 hour after the introduction of ozone to the chamber. Chamber air was collected for 30 minutes at 15 L min⁻¹, resulting in a total volume collected of 450 L. One quarter of the filter was extracted in 2 mL methanol (LC-MS grade, Fisher Scientific) using a vortex mixer. 2 mL water (LC-MS grade, Fisher Scientific) and 0.1 % by volume formic acid was added to the extract, which was analysed by direct infusion nano-ESI (Advion Triversa Nanomate) MS with a back pressure of 0.8 psi and an ionisation potential difference of -1.4 kV.

10 2.5 Ultra-high resolution MS operation and data analysis

The EESI and nanoESI sources were coupled to an ultra-high resolution mass spectrometer (Thermo Scientific LTQ Orbitrap Velos). Mass spectra were acquired in the range m/z 100-500 with mass accuracy <1.5 ppm and resolution of 100 000 (full width at half maximum, FWHM) at m/z 400. These characteristics mean that unambiguous molecular formula assignments for reaction product ions can be routinely achieved.

Mass spectra generated from EESI and offline nanoESI samples were analysed using a method similar to that described in Zielinski et al., (2017). Briefly, possible formulae were assigned to the spectra using XCalibur 2.1 software (Thermo Scientific). Evaluation of these initial assignments was performed using an in-house code run in Mathematica 10 (Wolfram Research Inc.). This removes formulae which fall outside a 2 ppm mass tolerance which removed formulae and those deemed implausible based on their atomic ratios. By strictly limiting permitted elements, we reduce the number of erroneous permutations of formulae that coincide with the measured m/z . Based on the oxygenated VOCs expected for α -pinene SOA (Table 2), we retained assignments containing only carbon, hydrogen and oxygen, and permitted sodium adduct formation in positive ion mode. Nitrogen-containing compounds are not expected to form via ozonolysis, but we note that this treatment excludes possible $[M + NH_4]^+$ adducts derived from the ammonium sulfate seed particles. However, in the raw data, such clusters were not apparent for major positive mode species such as pinonaldehyde. Following this assignment, the blank spectrum was subtracted and low intensity peaks deemed to fall below the noise of the Orbitrap instrument were removed to yield the final spectra.

Time series of individual particle-phase ions were also extracted from Xcalibur. These raw time series were processed by removing the transitions between sample and blank periods (~0.5 minutes),

Formatted: Subscript

Formatted: Superscript

averaging the intensity of the remaining sample period, and subtracting the averaged blank intensity for the minute preceding each sample. The resulting data points, with 7 minute time resolution, were shifted in time to account for the delay between sampling from the chamber and detection by EESI-MS. Uncertainties on the MS intensities represent the combined standard deviation of the sample and blank signals.

2.6 PTR-MS operation and data analysis

Gas phase VOC concentrations were measured using a proton transfer reaction mass spectrometer (PTR-ToF-MS 8000, Ionicon Analytik, Innsbruck, Austria) in the range m/z 10-500 and with a time resolution of 10 s. Parameters of the PTR-MS during the experiments were as follows: drift tube voltage: 600 V, drift tube pressure \approx 2.20 mbar, drift tube temperature: 60 °C, resulting in an E/N of ca. 135 Td (1 Td = 10^{-17} V cm²). Resolution in the Time-of-Flight (ToF) detector was 5000 (FWHM) at the mass of protonated acetone during all experiments. The MS inlet (PEEK tube, 60 °C, flow rate 0.1 L min⁻¹) was connected to the smog chamber with a 1mm inner diameter PTFE tube at room temperature.

Data analysis for the PTR-MS was carried out using PTR-MS Viewer 3.2 (Ionicon Analytik). Mass calibration has been adjusted using H₃¹⁸O⁺ (m/z = 21.023), NO⁺ (m/z = 29.998) and C₃H₇O⁺ (m/z = 59.049) as references. For all the compounds, concentrations were estimated on the basis of the rate constant (k) of the proton transfer reaction (Lindinger et al., 1998) which is essentially limited by gas-phase diffusion. Because the proton transfer reaction rate constants are not known for all compounds, a default rate constant (k) of 2×10^{-9} cm³ molecule⁻¹ s⁻¹ was used for those compounds without a measured rate constant. [Exothermic proton transfer reactions occur at a rate close to the collision limit](#) (Blake et al., 2009) [and known rate constants for a variety of VOCs are within 50 % of this value](#) (Smith and Spanel, 2005).

2.7 Numerical modelling of chamber chemistry

The complete reaction scheme for the degradation of α -pinene was extracted from the Master Chemical Mechanism (MCM) v3.3.1 (Jenkin et al., 1997; Saunders et al., 2003) via the MCM website (<http://mcm.leeds.ac.uk/MCM>) and used to simulate the ozone-initiated oxidation of α -pinene in the chamber. The reaction scheme was modified to approximate the introduction of ozone over the initial minutes of our experiments – an ozone precursor ~~with initial concentration~~ $[O_2]_{max}$

(from Table 1) was added to the mechanism and converted to ozone on the appropriate timescale (3-30 minutes). The initial precursor concentrations were selected to reproduce $[O_3]_{max}$ from Table 1. See the Supplement for more details about the chemical mechanism used.

- 5 Simulations were performed using the box model AtChem (<https://atchem.leeds.ac.uk>) via a web interface which enables the use of MCM mechanisms and relevant input parameters from the chamber. AtChem uses the Fortran CVODE library to integrate the MCM reaction scheme ODEs forward in time from the initial input conditions.
- 10 AtChem simulates gas-phase chemistry, but not aerosol formation. To compare gas-phase concentrations from the simulation with EESI-MS aerosol measurements, we neglected possible in-particle chemistry and focused on major aerosol components from previous studies [referenced in Table 2](#). Gas-particle partitioning considerations are discussed in section 3.3.2. The AtChem output concentrations (molecules cm^{-3}) were converted to parts per billion by volume (ppb) for comparison to PTR-MS measurements and $\mu\text{g m}^{-3}$ for aerosol species.
- 15

3. Results

3.1 Relative quantification of organic analytes in mixed organic-inorganic particles

- EESI-MS approaches have demonstrated excellent tolerance to very complex sample matrices compared to direct ESI-MS (Chen et al., 2006). Here we investigate the possible impact of inorganic salts on the EESI-MS intensities of organic ions in mixed aerosol particles. [Specifically, we establish the potential impact of inorganic seed particles on the relative quantification of organic acids \(detected as \$\[M-H\]^-\$ \) in the chamber experiments which follow.](#) Measurements quantifying the response of the technique to particles containing known mixtures of tartaric acid (TA) and ammonium sulfate (AS) are given in Figure 2. [TA is a highly oxygenated compound which is a relevant proxy for species present in aged organic aerosols. Its high water solubility and negligible volatility allow mixed TA-AS particles with precisely known composition to be prepared from solution.](#) Tartaric acid was detected as an $[M-H]^-$ ion in negative ion mode at m/z 149.0092. The intensity of this ion is plotted as a function of tartaric acid aerosol mass concentration, calculated from the total aerosol mass concentration and the tartaric acid mass fraction, in Figure 2.
- 20
- 25
- 30

Formatted: Superscript

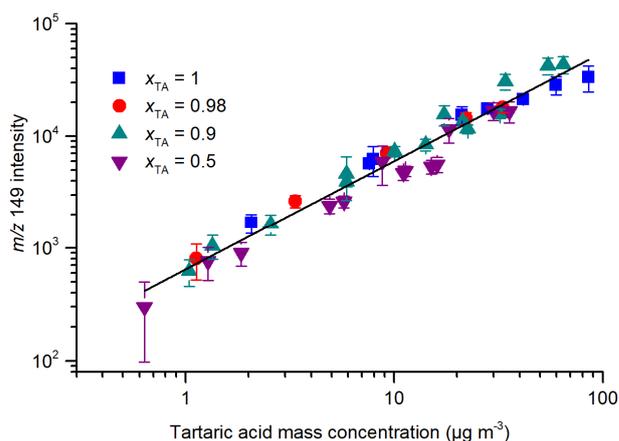


Figure 2: Intensity of m/z 149.0092 in negative ion mode, assigned to deprotonated tartaric acid, as a function of tartaric acid mass concentration in the aerosol. Particles were produced by nebulising bulk solutions containing varying proportions of tartaric acid and ammonium sulfate. The mole fraction of tartaric acid was varied between 0.5 and 1. Error bars represent the standard deviation of the MS signal over the 1 minute averaging time.

As for the single-component aerosol in Gallimore and Kalberer (2013), the detected mass spectrum signal intensity scales linearly with the organic aerosol mass concentration, this time over a range of organic/inorganic aerosol fractions. The best fit curve for the entire dataset in [Figure 2](#) follows a power law with an exponent of 0.97, close to the value of 1 expected for such a linear relationship.

The data in Figure 2 are colour coded according to the mole fraction of tartaric acid present, x_{TA} . To a good approximation, the data for different x_{TA} , and hence different x_{AS} , cluster around a common best fit curve suggesting that the different mass fractions of ammonium sulfate do not influence the ionisation efficiency (IE) of tartaric acid. There is limited evidence that higher concentrations of ammonium sulfate may suppress the organic signal; the data with $x_{TA} = x_{AS} = 0.5$ often fall slightly below the best fit curve. Figure S3 suggests that this suppression may result in a signal up to 25% lower than expected at the highest ammonium sulfate concentrations used.

This is not problematic for the current application because the conditions used in the chamber experiments when EESI-MS measurements were made involved low ammonium sulfate

Formatted: Normal, Line spacing: single

concentrations ($\sim 5 \mu\text{g m}^{-3}$) and high organic mole fractions ($x_{\text{org}} > 0.7$). Although care may be required if using substantially higher salt concentrations (or higher x_{salt}) in future studies, the potential suppression effect seems rather limited over the range tested. In this study, we further investigate the relative quantification of individual organic species during the growth of α -pinene SOA on ammonium sulfate seeds in section 3.3.2.

3.2 Molecular characterisation of α -pinene oxidation products

3.2.1 Assignment and comparison of EESI-MS and PTR-MS spectra

EESI-MS (particle phase) and PTR-MS (gas phase) were deployed during dark α -pinene ozonolysis experiments in the CASC chamber. Our EESI source was operated in both positive (+) and negative (-) ionisation modes for the first time which can help to identify complementary compound classes. A summary of the most abundant species identified during the “medium” concentration experiments (100 ppb α -pinene) is presented in Table 2. Full mass spectra are also shown in Figure S4 for reference. The low mass thresholds of the EESI-MS and PTR-MS mass analysers were m/z 100 and 10 respectively in this study. In total, ~ 400 ions were detected via PTR-MS including product parent ions, fragments and contaminants. >1000 ions were detected in both EESI-MS polarities, with 95 assignments retained in EESI(+), and 87 in EESI(-), following data treatment.

Formatted: Font: Italic

Neutral Mass (Da)	Formula	Possible assignment	PTR-MS ions	EESI-MS ions
136.1252	$\text{C}_{10}\text{H}_{16}$	α -pinene ^{a,b}	$[\text{M}+\text{H}]^+$; $[\text{C}_6\text{H}_8+\text{H}]^+$	ND
140.0837	$\text{C}_8\text{H}_{12}\text{O}_2$	2,2-dimethyl-cyclobutyl-1,3diethanal ^c	$[\text{M}+\text{H}]^+$	$[\text{M}+\text{H}]^+$; $[\text{M}+\text{Na}]^+$; $[\text{M}-\text{H}]^-$
140.1201	$\text{C}_9\text{H}_{16}\text{O}$	1-acetyl-2,2,3-trimethylcyclobutane ^c	$[\text{M}+\text{H}]^+$	$[\text{M}+\text{H}]^+$; $[\text{M}-\text{H}]^-$
154.0994	$\text{C}_9\text{H}_{14}\text{O}_2$	Norpinaldehyde ^{e,f}	$[\text{M}+\text{H}]^+$	$[\text{M}+\text{H}]^+$; $[\text{M}+\text{Na}]^+$; $[\text{M}-\text{H}]^-$
158.0943	$\text{C}_8\text{H}_{14}\text{O}_3$	2,2-dimethyl-3-formyl-acyclobutylmethanoic acid ^e	ND	$[\text{M}+\text{Na}]^+$; $[\text{M}-\text{H}]^-$

168.1150	C ₁₀ H ₁₆ O ₂	Pinonaldehyde ^{a,b,c,e,f}	[M+H] ⁺ ; [M-H ₂ O+H] ⁺ ; [C ₈ H ₁₀ +H] ⁺	[M+H] ⁺ ; [M+Na] ⁺ ; [M-H ₂ O+H] ⁺
170.0943	C ₉ H ₁₄ O ₃	Pinolic-3-acid ^{e,f}	[M+H] ⁺	[M+Na] ⁺ ; [M-H] ⁻
172.0743	C ₈ H ₁₂ O ₄	Terpenylic acid ^{c,d,g}	[M+H] ⁺	[M+H] ⁺ ; [M+Na] ⁺ ; [M-H] ⁻
182.0943	C ₁₀ H ₁₄ O ₃	Oxopinonaldehyde ^c	[M+H] ⁺	[M+H] ⁺ ; [M+Na] ⁺ ; [M-H] ⁻
184.1099	C ₁₀ H ₁₆ O ₃	Pinonic acid ^{c,d,e,f}	[M+H] ⁺	[M+H] ⁺ ; [M+Na] ⁺ ; [M-H] ⁻
186.0892	C ₉ H ₁₄ O ₄	Pinic acid ^{c,d,e,f}	[M+H] ⁺	[M+H] ⁺ ; [M+Na] ⁺ ; [M-H] ⁻
188.0685	C ₈ H ₁₂ O ₅	2-hydroxyterpenylic acid ^{c,g}	ND	[M-H] ⁻
200.1049	C ₁₀ H ₁₆ O ₄	OH-pinonic acid ^{c,d,e,f}	[M+H] ⁺	[M+Na] ⁺ ; [M-H] ⁻
232.0947	C ₁₀ H ₁₆ O ₆	Diaterpenylic acid acetate ^{c,d,g}	ND	[M+Na] ⁺ ; [M-H] ⁻
358.1628	C ₁₇ H ₂₆ O ₈	Pinylyl-diterpenylic ester ^d	ND	[M-H] ⁻

Table 2: Tentative assignments of a selection of major ions detected by PTR-MS and EESI-MS during dark α -pinene ozonolysis experiments with 100 ppb α -pinene precursor. ND = not detected. Compounds assigned in other studies were used to provide possible assignments here: a – Wisthaler et al., (2001); b – Lee et al., (2006); c – Hall IV and Johnston (2012); d – Kristensen et al., (2013), e – Jenkin (2004), f – Camredon et al., (2010), g – Claeys et al., (2009).

5

The major products identified by EESI-MS and PTR-MS following data treatment compare well to previous literature. Assigning PTR-MS spectra is slightly complicated by fragmentation; abundant products such as pinonaldehyde appear mostly as fragment ions (Wisthaler et al., 2001). Since fragmentation patterns for most VOCs are not known, we have not assigned ions $< m/z$ 100 aside from known major species reported in Blake et al., (2009). However, we present all detected PTR-MS ions in Figure S4.

10

A positive characteristic of EESI-MS is that most species are detected as intact quasi-molecular ions (Table 2). Furthermore, the two ion polarities allow detection of complementary compound classes. EESI(+) mostly forms H⁺ and Na⁺ clusters with the parent molecule and enables a wide range of functional groups (carbonyls, alcohols, carboxylic acids) to be detected (Table 2). Doezema et al., (2012) reported that [M-H₂O+H]⁺ fragment ions of major products such as pinonic acid and pinonaldehyde were more abundant than corresponding [M+H]⁺ peaks. We found that such


15

fragments were minor compared to quasi-molecular ions, and not observed for many species. This suggests that the choice of EESI ~~parameters conditions, such as a lower spray voltage in the current study,~~ may be an important determinant of fragmentation. Negative ionisation is a more specific technique which mostly deprotonates acidic functional groups and so carboxylic acids (including multifunctional species) are readily detected as $[M - H]^-$ ions.

Taken together, EESI(-)-MS, EESI(+)-MS and PTR-MS enable the detection of a wide range of typical SOA components and gas-phase oxidation products with different volatilities and polarities. We illustrate this using the two dimensional formulation introduced by Kroll et al., (2011). This calculates a compound's average carbon oxidation state, \overline{OS}_c , as a metric for its degree of oxidation. For molecules containing only carbon, hydrogen and oxygen:

$$\overline{OS}_c = \frac{2n_O}{n_C} - \frac{n_H}{n_C} \quad (1)$$

Where n_O , n_C and n_H are the number of oxygen, carbon and hydrogen atoms respectively. This expression is exact unless oxygen is present in peroxide or other functional groups with oxidation state $\neq 2$. Figure 3 shows calculated \overline{OS}_c from PTR, EESI(+) and EESI(-) MS assignments as a function of n_C . Many PTR-MS ions from Figure S4 are not assigned to formulae and therefore not included in Figure 3.

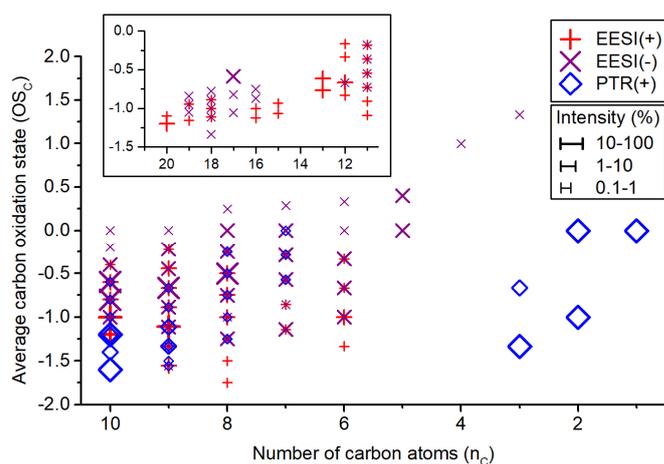

5 **Figure 3:** The average carbon oxidation state of compounds detected via EESI-MS and PTR-MS as a function of n_c . Spectra were acquired ~1 hour after the start of ozone introduction for the “medium” concentration experiments. Marker size is **proportional to the logarithm of related to the MS intensity according to the size bins indicated on the figure**. The inset plot shows oligomeric species ($n_c > 10$) **with a constant marker size for clarity**. No PTR-MS signals with $n_c > 10$ were detected.

The ensemble average \overline{OS}_c for particle-phase products resulting from monoterpene ozonolysis is quoted as -1.1 to -0.5 in Kroll et al. (2011) based on ESI-MS and Aerosol Mass Spectrometer (AMS) literature, in good agreement with our EESI(+)(-)-MS observations. Within this ensemble average, however, the ions detected in the two ion polarities, and in the gas phase via PTR-MS, occupy different regions of the \overline{OS}_c - n_c space in Figure 3.


15 Aside from α -pinene, the products detected by PTR-MS with molecular formula assignments mainly fall into two categories: $n_c = 1-3$ species resulting from reactions which fragment the α -pinene carbon backbone, and $n_c = 8-10$ species such as pinonaldehyde resulting from functionalisation reactions. These larger species are sufficiently volatile that a fraction remains in the gas phase, which is reflected in their low average oxidation states ($\overline{OS}_c < -0.5$). However, many are condensable and therefore also detected in the particle phase via EESI(+), which is generally more sensitive to compounds with only carbonyl groups compared to EESI(-). EESI(+) ions mostly occupy a region with $-1.5 < \overline{OS}_c < -0.5$, with the most abundant ions assigned as semi-volatile carbonyls such as pinonaldehyde. Carboxylic acids and other functional groups are also present. In addition to

functionalisation products, oligomers from accretion reactions, and products resulting from radical-induced carbon backbone fragmentation, can also be detected.

Compounds detected via EESI(-)-MS were on average more oxidised than EESI(+)-MS and PTR-MS, and also possess a slightly higher average molecular weight (Figure S4). The negative ion mode is highly efficient at ionising carboxylic acid functional groups, and these heavier and more oxygenated species tend to condense most readily into the particle phase. A number of low n_C species and oligomers were also detected, again indicating that multiple generations of chemistry, including secondary OH-mediated fragmentation, was being assessed. We quantitatively compare EESI(-)-MS time series for three of the main condensable oxidation products (pinonic acid, pinic acid and OH-pinonic acid) with model simulations in section 3.3.2.

3.2.2 Comparison of online EESI(-) and offline nanoESI(-) mass spectra

Figure 4 shows a comparison in the same \overline{OS}_c-n_C space as Figure 3 between online measurements of particle composition via EESI(-)-MS and offline nanoESI(-)-MS analysis following the collection of SOA particles on to quartz fibre filters.

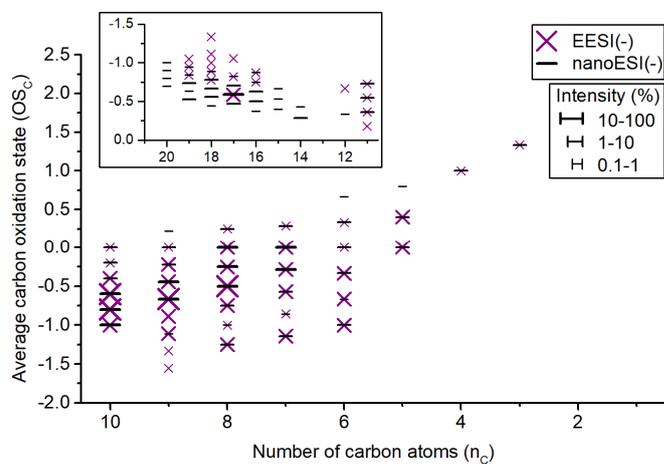


20 **Figure 4: A comparison of α -pinene SOA oxidation products detected using online EESI(-) and offline nanoESI(-) MS. The EESI(-)-MS spectrum acquisition and offline sampling period started ~1 hour after**
16

Formatted: Normal, Line spacing: single

the start of ozone introduction, for the “medium” concentration experiments. Marker size is proportional-related to the logarithm-of-the-MS intensity according to the size bins indicated on the figure. The inset plot shows oligomeric species ($n_c > 10$) with a constant marker size for clarity.

- 5 There is good agreement between the two data sets in Figure 4 in terms of the range of \overline{OS}_c and n_c detected, and the relative intensities of species in the main plot (indicated by marker size). Pinic acid ($n_c = 9$, $\overline{OS}_c = -0.67$) is the most abundant ion in EESI(-) and nanoESI(-), and essentially all monomeric compounds present with $\overline{OS}_c < 0$ are detected using both methodologies. A direct comparison of the mass spectra is provided in Figure S5. The major dimers reported in previous
- 10 studies (Hall IV and Johnston, 2012; Kristensen et al., 2013; Reinhardt et al., 2007) are also detected using both approaches here. Differences between EESI(-) and nanoESI(-) can be observed in two regions: firstly, a few oxidised monomers with $\overline{OS}_c > 0$ are detected only using the filter method. Secondly, the oligomers detected via nanoESI(-)-MS are more numerous, and generally more oxidised, than for EESI(-)-MS.

15

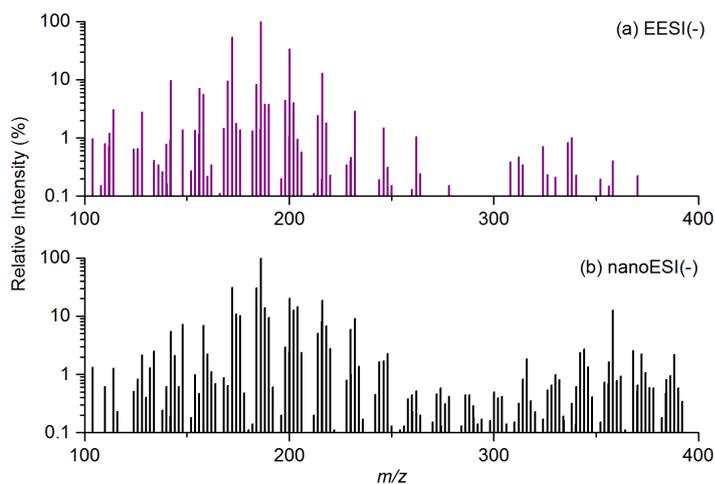

20

Figure 5: Mass spectra obtained during the dark ozonolysis of α -pinene under “medium” conditions (Table 1) using (a) online EESI-MS in negative ionisation mode and (b) nanoESI-MS of SOA filter extracts. The online MS was acquired and the filter collected 1 hour after the start of ozonolysis in the chamber. The spectra are very similar in the monomer region (< 250 Da), but the oligomers detected are more numerous and possess slightly higher molecular weights in the nanoESI(-) spectrum.

The peaks absent from EESI(-)-MS are generally the least abundant in the offline sampling method (Figure S5), so we suspect differences are mainly a consequence of sample pre-concentration and hence improved sensitivity using the filter sampling method. While the EESI source operates at an aerosol flow rate of $\sim 1 \text{ L min}^{-1}$, 450 L of chamber air is drawn through the filter for an offline sample. The capture efficiency of aerosols in the EESI process is also expected to be less efficient than extraction from a substrate. An alternative possibility is that offline collection and analysis introduces positive artefacts to the nanoESI(-)-MS spectrum, such as via additional reaction on the substrate. [Horan et al., \(2012\) found that the relative abundance of oligomers was also higher in filter samples than their online AESI method, which was attributed to a negative filter sampling artefact – evaporation of semi-volatile material \(predominantly monomers\) during collection.](#) However, the overall good agreement between the methods is encouraging and the use of both during the same experiment could provide the benefits of offline sampling (sensitivity) and online sampling (time resolution, relative quantification) together.

15

3.3 Temporal evolution of molecular composition during α -pinene oxidation

3.3.1 Time series of individual particle-phase ions

We now focus on the ability of our online MS techniques to monitor relative concentration changes of individual species during α -pinene oxidation. In particular, we monitor some of the major low volatility products in the particle phase using EESI(-)-MS. [Figure 6Figure-5](#) shows an illustrative raw time series from the “medium” experiment conditions for m/z 185.0819, assigned to $[\text{M} - \text{H}]^-$ for an abundant oxidation products, pinic acid (Table 2). We present the MS data in terms of ion intensities with alternating blank and sample measurements. The pinic acid intensity increases over the first hour of the experiment, as does the total aerosol mass (secondary y-axis in [Figure 6Figure-5](#)). Both signals tend towards a plateau at later times. Ions assigned to oxidation products in Table 2 show similar increases over time, although the precise time dependence varies depending on the product. We show blank-subtracted time series for other aerosol-phase products in the next section.

20
25

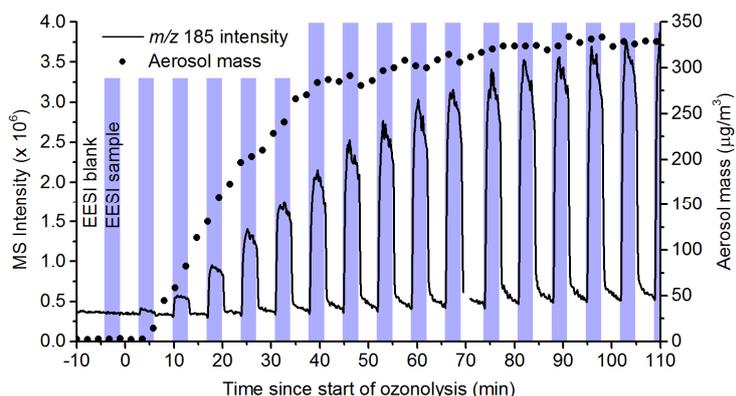


Figure 6: Left y-axis: Intensity of m/z 185.0819, corresponding to pinic acid, after the start of an α -pinene ozonolysis experiment. Right y-axis: Mass concentration of aerosol in the chamber. The measurements were made using the new EESI-MS batch sampling system (Figure 1). Blue bands correspond to sampling of chamber air from the reservoir volume (3.5 minutes) while the blanks in between correspond to clean air flushing (3.5 minutes). The MS discontinuity around 70 minutes corresponds to refilling of the primary EESI solvent syringe.

As configured, the sampling setup enables a blank and chamber measurement to be obtained in a seven minute cycle, a substantially higher time resolution than most other semi-continuous sampling methods (Bateman et al., 2009; Pereira et al., 2014) or collection onto filters. It is comparable to the recent highly time-resolved particle-into-liquid-sampling measurements of Zhang et al., (2015). The signal intensities vary by less than 15 % across a sample window (3.5 minutes) (Figure 6Figure-5), with most of the decrease attributed to particle deposition in the intermediate reservoir volume and sampling lines. An advantage of flushing the EESI source during each blank period is that baseline changes can be monitored and accounted for. The signals in Figure 6Figure-5 rapidly return towards the baseline recorded at the start of the experiment as the source is flushed. Small increases in this baseline (e.g. due to particle deposition in the source) are subtracted during data processing. Importantly, we avoid the major EESI source contamination problems reported in other applications (McCullough et al., 2011). We suspect this a combination of using relatively low analyte concentrations, the optimised source parameters from Gallimore and Kalberer (2013) and this regular flushing procedure.

The semi-volatile nature of SOA means that both gas- and particle-phase species will be present in the chamber. We examined whether gas-phase species contribute to our observed EESI(-)-MS

signal under the “medium” reaction conditions by removing particles from the sample flow using a HEPA filter (Figure 1). With particles filtered out, none of the species listed in Table 2 could be detected above levels observed for the solvent blanks. This was also the case even if the charcoal denuder in Figure 1, intended to remove gas-phase species, was bypassed.

5

The aerosol mass loading in the chamber ($\sim 300 \mu\text{g m}^{-3}$) would strongly bias most of the compounds in Table 2 towards the particle phase. For instance, the most abundant ion, pinic acid, has a vapour pressure $\sim 2 \mu\text{g m}^{-3}$ at 294 K (Bilde and Pandis, 2001), so $> 99\%$ would be expected to reside in the particle phase based on an absorptive partitioning argument (Pankow, 1994). This might explain the lack of detected species in the present SOA system. However, a number of studies have detected gas-phase species using an electrospray source, e.g. (Horan et al., 2012; Wu et al., 2000; Zhao et al., 2017a). The ion source design and operating parameters appear important in determining the ionisation efficiency and mechanism (uptake into droplets or gas-phase chemical ionisation). Future work to simultaneously detect semi-volatile species in both phases, and understand the relative efficiencies of gas- and particle-phase ionisation, is therefore merited.

10

15

Formatted: Superscript

3.3.2 Comparing measured and modelled time dependence of individual species

An important application of simulation chamber experiments is to better constrain and validate atmospheric reaction mechanisms, particularly for complex VOC chemistry. We compare here individual species measured during the chamber experiments using PTR-MS and EESI-MS to predictions from the AtChem chamber box model using the near-explicit α -pinene oxidation scheme from the Master Chemical Mechanism (referred to as “MCM simulations” from this point). We focus on the first hour of each experiment to assess how the techniques capture the time evolution of composition.

25

We first benchmark the simulations to measurements of $[\alpha\text{-pinene}]$ using PTR-MS, an established technique. Figure 7 shows the simulated and measured α -pinene concentrations in the chamber for experiments with $[\alpha\text{-pinene}]_0 = 45, 100$ and 500 ppb (referred to as low, medium and high respectively) and $[\text{O}_3]_{\text{max}}/[\alpha\text{-pinene}]_0 = 3$. Also shown on the secondary y-axis are the corresponding measured SOA concentrations.

30

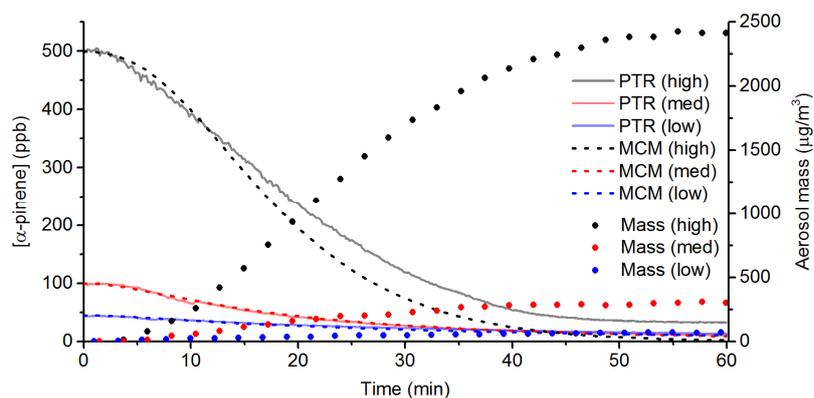


Figure 76: α -pinene loss and SOA production during chamber experiments with varying $[\alpha\text{-pinene}]_0$. Dashed lines: measured $[\alpha\text{-pinene}]$ from PTR-MS; Solid lines: MCM simulated $[\alpha\text{-pinene}]$; Points: measured aerosol mass from SMPS.

5

The “sigmoidal” shape of the α -pinene loss is a consequence of ozone being introduced over a finite period of up to 30 minutes at the start of the experiment, as discussed in section 2.2. The MCM generally performs well in simulating the observed α -pinene concentration, especially for the low and medium concentration conditions when the ozone introduction period was only a few minutes.



10

An expanded view of the low and medium experiments is provided in Figure S56. The largest discrepancy is for the high concentration experiment, where the simulated loss is more rapid than measured. We attribute this to the longer ozone introduction time in this experiment (~ 30 minutes) which will lead to a more uncertain chamber mixing state at the start of the experiment.

15

We now demonstrate a comparison of aerosol-phase EESI(-)-MS intensities to the MCM for individual species across the low, medium and high concentration conditions from Table 1. [Figure 8](#) shows time series for m/z 183.1027, m/z 185.0819 and m/z 199.0976, assigned as pinonic acid, pinic acid and OH-pinonic acid respectively (Table 2). The secondary y-axes show simulated concentrations of these species from the MCM under the corresponding conditions.

20

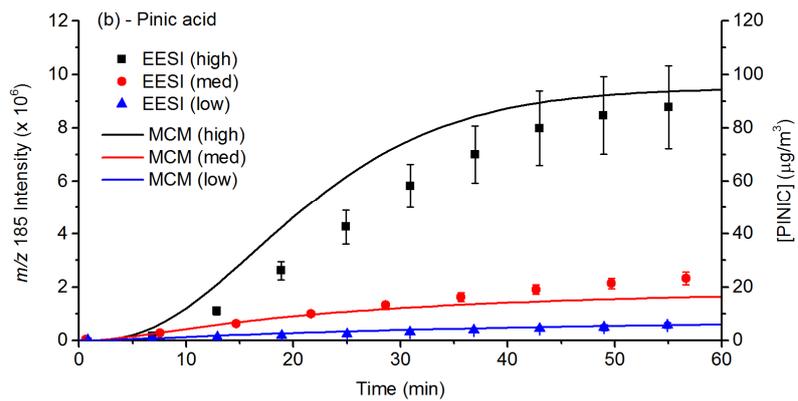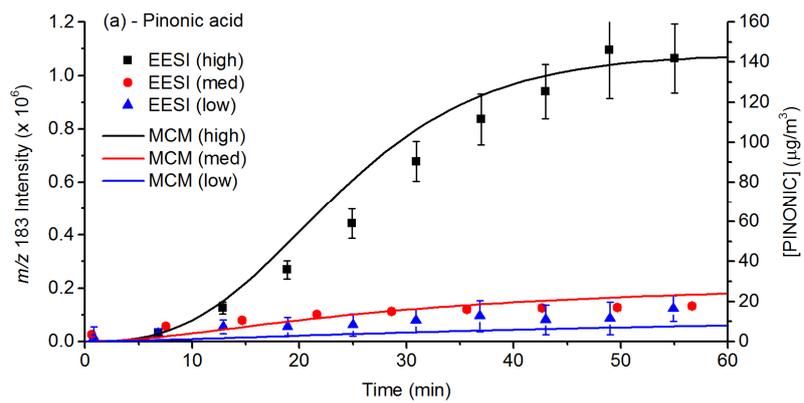

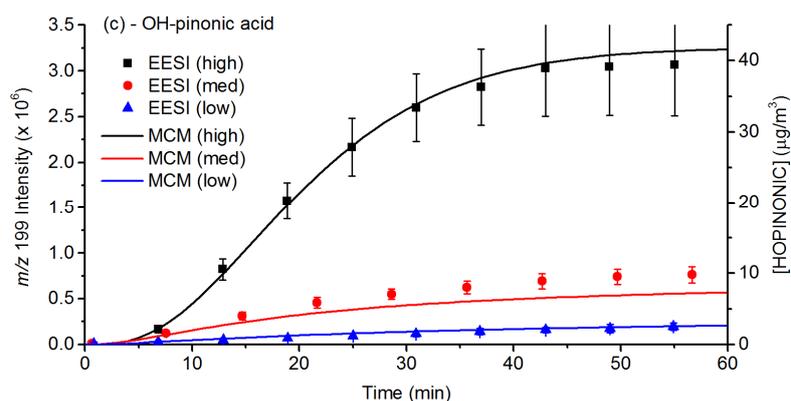


Figure 87: Comparison between EESI-MS intensities (left y-axis) and MCM simulated concentrations (right y-axis) for (a) pinonic acid, (b) pinic acid and (c) OH-pinonic acid during chamber experiments with different $[\alpha\text{-pinene}]_0$. MS intensities are absolute, following averaging and blank subtraction. The measurements and model agree closely both in terms of the time dependence of product formation and the relative yields under different reaction conditions.

The overall agreement between MS intensities and MCM simulations is very encouraging. The measurements and model compare well in two respects: the time dependence of product formation, and the relative concentrations of a given product in the low, medium and high conditions. Note that the MS intensities of the three compounds cannot be directly compared without calibration due to the species' different ionisation efficiencies (IEs).

The product time series reflect the rate of consumption of α -pinene in the chamber. As for α -pinene, a pronounced "sigmoidal" profile is observed and simulated for the high concentration conditions, and the slightly overpredicted α -pinene loss rate may explain the more rapid growth of pinonic acid and pinic acid in the model than measured. OH-pinonic acid is a close fit to the model under the range of conditions tested.

The individual product yields after 1 hour (when the α -pinene precursor has been almost completely consumed and timing uncertainties are less important) compare well between measurement and model and scale approximately with $[\alpha\text{-pinene}]_0$. Typically, these relative measured and modelled yields are self-consistent for a given product to within ~25 %, except for pinonic acid in the low

concentration experiment. The data for low and medium concentration time series are shown in more detail in Figure S67.


Although pinonic acid, pinic acid and OH-pinonic acid are reported as major particle-phase oxidation products in a range of studies (Table 2), the discussion above assumes that the gas-phase concentrations from the MCM are a good proxy for particle-phase concentrations assessed by EESI-MS. Particle-phase reactions are unlikely to be a large source or sink of these major products, although they may be important for a range of high molecular weight species (Camredon et al., 2010). The equilibrium partitioning of products between the gas and particle phases will favour the particle phase for pinic acid and OH-pinonic acid because their saturation concentrations (~5-10 $\mu\text{g m}^{-3}$, (Müller et al., 2012; Yatavelli et al., 2014)) are substantially lower than aerosol mass loadings (100-2400 $\mu\text{g m}^{-3}$) in our experiments.

Pinonic acid is thought to have a significantly higher saturation concentration (in the range 10^2 - 10^3 $\mu\text{g m}^{-3}$ depending on the temperature and estimation method used (Müller et al., 2012; Yatavelli et al., 2014)). Hence, it is expected to reside across both phases in our experiments. However, a few observations suggest that the aerosol phase is still favoured here. Gas phase concentrations estimated by PTR-MS are a small fraction of the corresponding MCM predictions in Figure 8Figure 7(a). The measured EESI-MS intensities also track the predicted MCM concentrations relatively well over time, even as the aerosol mass loading in the chamber is increasing substantially. Zhang et al., (2015) found that aerosol-phase concentrations of pinonic acid increased substantially at 50 % RH (similar to 60% here) compared to dry conditions, and a recent field study concluded that measured pinonic acid concentrations in the aerosol exceeded absorptive partitioning predictions by a factor of ~ 20 (Yatavelli et al., 2014). Given the relatively high predicted Henry's law coefficient of pinonic acid (~ 2×10^7 M atm^{-1} , (Lignell et al., 2013)), it may be that the presence of aerosol liquid water enhances uptake into the aerosol phase. As for all products in our study, structural isomers of the assignments in Table 2 may also be present as isobaric ions in our mass spectra.

Despite the potential limitations of this comparison, Figure 8Figure 7 provides further evidence that EESI-MS can be used for relative quantification of individual species in organic aerosols. Moreover, it extends this applicability to scenarios where the particles contain a complex mixture of components, and where the particle composition, size and total mass are evolving. Specifically, we have demonstrated here that the influence of the bulk aerosol "matrix" on EESI ionisation appears to be negligible up to SOA loadings of ~2400 $\mu\text{g m}^{-3}$ and that the EESI mechanism can tolerate small quantities of inorganic material. The time evolution is also well captured for much lower analyte

concentrations of a few $\mu\text{g m}^{-3}$ (Figure S78(c)). This is a significant advantage compared to conventional direct infusion ESI-MS, where ion intensities are typically only used as a qualitative indicator, if at all, due to strong matrix effects.

5 Figure 9 shows the measured EESI(-)-MS signal plotted against the corresponding simulated concentration at that time for OH-pinonic acid, which shows the best correlation in time between measurement and model of the three compounds discussed in Figure 8. This relationship is linear over orders of magnitude in concentration, and regions where the concentrations coincide (e.g. the initial point of the “high” experiment with later points in the “low” and “medium” experiments) overlap well. Figure S78 shows an illustrative plot for all three species from Figure 7, using only the concentrations around 1 hour to minimise timing uncertainties discussed above.

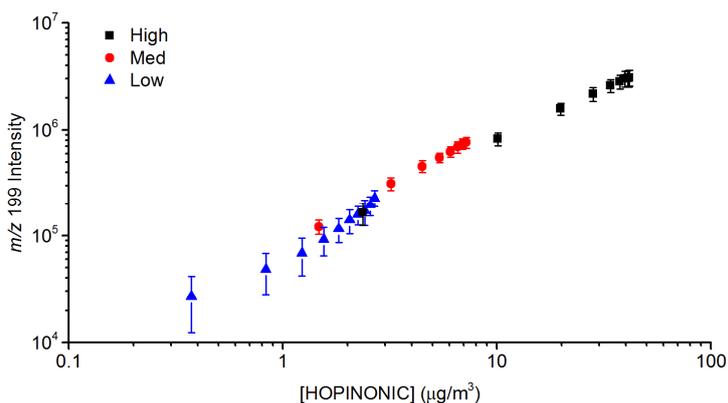

15 Figure 98: Correlation between MS intensity and MCM mass across three different experiments for OH-pinonic acid.

This representation is analogous to the plots for tartaric acid shown in Figure 2, except that the MS signal is compared to the model rather than a known analyte concentration. In principle, a direct calibration curve such as Figure 2 would allow MS intensities to be converted to absolute concentrations for any species where authentic standards are available. In practice, however, the number of species present in aerosols, and the general unavailability of suitable standards, makes this approach impractical for routine quantification. Comparison to modelled concentrations in this way may therefore provide an approximate indicator of ionisation efficiency for a range of different

species in aerosols. However, as discussed above, care is required in interpreting aerosol-phase concentration changes for the many species where in-particle reaction or gas-particle partitioning may be significant. A coupled model of aerosol and gas phase chemistry (Gallimore et al., 2017a; Shiraiwa et al., 2010) would therefore be a desirable tool to use alongside future chamber
5 experiments.

4. Conclusions

Online measurements of particle and gas phase chemistry in the new Cambridge Atmospheric Simulation Chamber (CASC) have been achieved simultaneously using complementary “soft” ionisation mass spectrometry techniques: Extractive Electrospray Ionisation (EESI) and Proton
10 Transfer Reaction (PTR). The results for EESI-MS are encouraging and prompt continuing use and further development of the technique in future. Its principle advantages over conventional electrospray techniques are (1) the sample and blank measurements are obtained online, providing highly time resolved information with fewer potential artefacts, and (2) that the ion intensities can be used as a relative measure of concentration due to the lack of matrix interference, and in principle
15 converted to an absolute concentration via calibration.

The lack of matrix interference in EESI-MS compared to direct ESI-MS has been noted in other applications. The mechanistic differences are not fully understood, but a likely rationale is that the primary electrospray conditions are constant during EESI, but vary substantially depending on the
20 dissolved analytes in direct ESI. Our work (here and in previous studies) shows a correlation between MS signal and total analyte mass which does not appear to saturate at the upper end of the concentration range tested ($\sim 2400 \mu\text{g m}^{-3}$). This implies there is an excess of primary charged droplets available to extract and ionise the aerosol components, and hence that the MS intensity of each analyte depends on its relative ionisation efficiency, which has been modelled as a function of
25 a species’ ionisation in solution and ability to delocalise charge (Kruve et al., 2014). Our limited tests with this EESI-MS configuration show that the signal arising is a result of droplet-particle collisions, with negligible contribution from gas-phase analytes. Further insight into the EESI mechanism may be obtained by assessing when and how MS saturation behaviour occurs at higher mass loadings.

30 Improving EESI-MS sensitivity would be an advantage in future atmospheric chemistry applications. The downside of our Orbitrap mass spectrometer is that the instrument’s ion collection

and transmission properties are less efficient relative to other instruments. Coupling the EESI ion source to an alternative mass analyser is an area of active investigation. Pre-concentrating the airborne particles using a virtual impactor system similar to Vogel et al., (2013) may also provide an order-of-magnitude boost to sensitivity.

5

Although out of the scope of the current study, our molecular composition measurements from the chamber may be amenable to detailed process modelling. A model which includes descriptions of gas-particle partitioning, alongside reactions in both phases, may be better able to capture the dynamic evolution of particle phase components and probe multiphase processing and extended aging of the initial products.

10

Supplementary information

The supplement contains details related to operation of the atmospheric chamber and EESI sampling system, [further details about MCM modelling](#), full EESI-MS ~~and~~, PTR-MS ~~and offline nanoESI-MS~~ spectra, and additional figures comparing the online MS measurements to MCM simulations.

15 Acknowledgements

This work was funded by the European Research Council (grant 279405), the UK Natural Environment Research Council (grant NE/H52449X/1) and the Velux foundation (project number 593).

Data access

20 Data presented in this study can be obtained by contacting the corresponding author.

References

Aiken, A. C., Decarlo, P. F., Kroll, J. H., Worsnop, D. R., Huffman, J. A., Docherty, K. S., Ulbrich, I. M., Mohr, C., Kimmel, J. R., Sueper, D., Sun, Y., Zhang, Q., Trimborn, A., Northway, M. J., Ziemann, P. J., Canagaratna, M. R., Onasch, T. B., Alfarra, M. R., Prevot, A. S. H., Dommen, J.,
25 Duplissy, J., Metzger, A., Baltensperger, U. and Jimenez, J. L.: O / C and OM / OC Ratios of Primary , Secondary , and Ambient Organic Aerosols with High-Resolution Time-of-Flight Aerosol Mass

- Spectrometry, *Environ. Sci. Technol.*, 42(12), 4478–4485, 2008.
- Bateman, A. P., Nizkorodov, S. A., Laskin, J. and Laskin, A.: Time-resolved molecular characterization of limonene/ozone aerosol using high-resolution electrospray ionization mass spectrometry, *Phys. Chem. Chem. Phys.*, 11(36), 7931–7942, doi:10.1039/b916865f, 2009.
- 5 Bateman, A. P., Nizkorodov, S. A., Laskin, J. and Laskin, A.: High-Resolution Electrospray Ionization Mass Spectrometry Analysis of Water-Soluble Organic Aerosols Collected with a Particle into Liquid Sampler, *Anal. Chem.*, 82(19), 8010–8016, 2010.
- Bilde, M. and Pandis, S. N.: Evaporation Rates and Vapor Pressures of Individual Aerosol Species Formed in the Atmospheric Oxidation of alpha- and beta-Pinene, *Environ. Sci. Technol.*, 35(16),
10 3344–3349, 2001.
- Blake, R. S., Monks, P. S. and Ellis, A. M.: Proton-transfer reaction mass spectrometry., *Chem. Rev.*, 109(3), 861–96, doi:10.1021/cr800364q, 2009.
- Boucher, O., Randall, D., Artaxo, P., Bretherton, C., Feingold, G., Forster, P., Kerminen, V.-M., Kondo, Y., Liao, H., Lohmann, U., Rasch, P., Satheesh, S. K., Sherwood, S., Stevens, B. and Zhang,
15 X. Y.: Clouds and Aerosols, in *Climate Change 2013: The Physical Science Basis. Contribution of Working Group I to the Fifth Assessment Report of the Intergovernmental Panel on Climate Change*, edited by T. F. Stocker, D. Qin, G.-K. Plattner, M. Tignor, S. K. Allen, J. Boschung, A. Nauels, Y. Xia, V. Bex, and P. M. Midgley., 2013.
- Brüggemann, M., Karu, E., Stelzer, T. and Hoffmann, T.: Real-time analysis of ambient organic
20 aerosols using aerosol flowing atmospheric-pressure afterglow mass spectrometry (AeroFAPA-MS), *Environ. Sci. Technol.*, 49(9), 5571–5578, doi:10.1021/es506186c, 2015.
- Camredon, M., Hamilton, J. F., Alam, M. S., Wyche, K. P., Carr, T., White, I. R., Monks, P. S., Rickard, A. R. and Bloss, W. J.: Distribution of gaseous and particulate organic composition during dark alpha-pinene ozonolysis, *Atmos. Chem. Phys.*, 10, 2893–2917, doi:10.5194/acpd-9-27837-
25 2009, 2010.
- Chen, H., Venter, A. and Cooks, R. G.: Extractive electrospray ionization for direct analysis of undiluted urine, milk and other complex mixtures without sample preparation, *Chem. Commun.*, (19), 2042–4, doi:10.1039/b602614a, 2006.
- Chhabra, P. S., Flagan, R. C. and Seinfeld, J. H.: Elemental analysis of chamber organic aerosol
30 using an aerodyne high-resolution aerosol mass spectrometer, *Atmos. Chem. Phys.*, 10, 4111–4131, doi:10.5194/acp-10-4111-2010, 2010.
- Claeys, M., Iinuma, Y., Szmigielski, R., Surratt, J. D., Blockhuys, F., van Alsenoy, C., Bogen, O., Sierau, B., Gomez-Gonzalez, Y., Vermeylen, R., van der Veken, P., Shahgholi, M., Chan, A. W. H.,

- Herrmann, H., Seinfeld, J. H. and Maenhaut, W.: Terpenylic Acid and Related Compounds from the Oxidation of alpha-Pinene : Implications for New Particle Formation and Growth above Forests, *Environ. Sci. Technol.*, 43(18), 6976–6982, 2009.
- Clark, C. H., Nakao, S., Asa-Awuku, A., Sato, K. and Cocker, D. R.: Real-Time Study of Particle-Phase Products from α -Pinene Ozonolysis and Isoprene Photooxidation Using Particle into Liquid Sampling Directly Coupled to a Time-of-Flight Mass Spectrometer (PILS-ToF), *Aerosol Sci. Technol.*, 47(12), 1374–1382, doi:10.1080/02786826.2013.844333, 2014.
- Cocker, D. R., Flagan, R. C. and Seinfeld, J. H.: State-of-the-art chamber facility for studying atmospheric aerosol chemistry, *Environ. Sci. Technol.*, 35(12), 2594–2601, doi:10.1021/es0019169, 2001.
- Devenport, N. A., Blenkhorn, D. J., Weston, D. J., Reynolds, J. C. and Creaser, C. S.: Direct Determination of Urinary Creatinine by Reactive-Thermal Desorption-Extractive Electrospray-Ion Mobility-Tandem Mass Spectrometry., , 357–361, 2014.
- Doezema, L. A., Longin, T., Cody, W., Perraud, V., Dawson, M. L., Ezell, M. J., Greaves, J., Johnson, K. R. and Finlayson-Pitts, B. J.: Analysis of secondary organic aerosols in air using extractive electrospray ionization mass spectrometry (EESI-MS), *RSC Adv.*, 2(7), 2930, doi:10.1039/c2ra00961g, 2012.
- Dominici, F., Peng, R. D., Bell, M. L., Pham, L., McDermott, A., Zeger, S. L. and Samet, J. M.: Fine particulate air pollution and hospital admission for cardiovascular and respiratory diseases., *J. Am. Med. Assoc.*, 295(10), 1127–34, doi:10.1001/jama.295.10.1127, 2006.
- Edney, E. O., Kleindienst, T. E., Jaoui, M., Lewandowski, M., Offenber, J. H., Wang, W. and Claeys, M.: Formation of 2-methyl tetrols and 2-methylglyceric acid in secondary organic aerosol from laboratory irradiated isoprene/NOX/SO₂/air mixtures and their detection in ambient PM_{2.5} samples collected in the eastern United States, *Atmos. Environ.*, 39(29), 5281–5289, doi:10.1016/j.atmosenv.2005.05.031, 2005.
- Gallimore, P. J. and Kalberer, M.: Characterizing an extractive electrospray ionization (EESI) source for the online mass spectrometry analysis of organic aerosols, *Environ. Sci. Technol.*, 47(13), 7324–31, doi:10.1021/es305199h, 2013.
- Gallimore, P. J., Griffiths, P. T., Pope, F. D., Reid, J. P. and Kalberer, M.: Comprehensive modeling study of ozonolysis of oleic acid aerosol based on real-time, online measurements of aerosol composition, *J. Geophys. Res. Atmos.*, 122, 4364–4377, doi:10.1002/2016JD026221, 2017a.
- Gallimore, P. J., Mahon, B. M., Wragg, F. P. H., Fuller, S. J., Giorio, C., Kourtchev, I. and Kalberer, M.: Multiphase composition changes and reactive oxygen species formation during limonene

- oxidation in the new Cambridge Atmospheric Simulation Chamber (CASC), *Atmos. Chem. Phys. Discuss.*, In review, doi:doi:10.5194/acp-2017-186, 2017b.
- Goldstein, A. H. and Galbally, I. E.: Known and Unexplored Organic Constituents in the Earth's Atmosphere, *Environ. Sci. Technol.*, 41, 1515–1521, 2007.
- 5 Guenther, A. B., Jiang, X., Heald, C. L., Sakulyanontvittaya, T., Duhl, T., Emmons, L. K. and Wang, X.: The Model of Emissions of Gases and Aerosols from Nature version 2.1 (MEGAN2.1): an extended and updated framework for modeling biogenic emissions, *Geosci. Model Dev.*, 5, 1471–1492, doi:10.5194/gmd-5-1471-2012, 2012.
- Hall IV, W. A. and Johnston, M. V.: Oligomer formation pathways in secondary organic aerosol
10 from MS and MS/MS measurements with high mass accuracy and resolving power, *J. Am. Soc. Mass Spectrom.*, 23(6), 1097–1108, doi:10.1007/s13361-012-0362-6, 2012.
- Hallquist, M., Wenger, J. C., Baltensperger, U., Rudich, Y., Simpson, D., Claeys, M., Dommen, J., Donahue, N. M., George, C., Goldstein, A. H., Hamilton, J. F., Herrmann, H., Hoffmann, T., Iinuma, Y., Jang, M., Jenkin, M. E., Jimenez, J. L., Kiendler-Scharr, A., Maenhaut, W., McFiggans, G.,
15 Mentel, T. F., Monod, A., Prévôt, A. S. H., Seinfeld, J. H., Surratt, J. D., Szmigielski, R. and Wildt, J.: The formation, properties and impact of secondary organic aerosol: current and emerging issues, *Atmos. Chem. Phys.*, 9, 5155–5236, 2009.
- Hoffmann, T., Huang, R.-J. and Kalberer, M.: Atmospheric Analytical Chemistry, *Anal. Chem.*, 83(12), 4649–64, doi:10.1021/ac2010718, 2011.
- 20 Horan, A. J., Gao, Y., Hall, W. A. and Johnston, M. V.: Online Characterization of Particles and Gases with an Ambient Electrospray Ionization Source, *Anal. Chem.*, 84, 9253–9258, 2012.
- Husar, R. B., Holloway, J. M. and Patterson, D. E.: Spatial and temporal pattern of eastern U.S. haziness: A summary, *Atmos. Environ.*, 15, 1919–28, doi:10.1016/0004-6981(81)90226-2, 1981.
- Jenkin, M. E.: Modelling the formation and composition of secondary organic aerosol from α - and
25 β -pinene ozonolysis using MCM v3, *Atmos. Chem. Phys.*, 3(3), 1741–1757, 2004.
- Jenkin, M. E., Saunders, S. M. and Pilling, M. J.: The Tropospheric Degradation of Volatile Organic Compounds: A Protocol for Mechanism Development, *Atmos. Environ.*, 31(1), 81–104, 1997.
- Jimenez, J. L., Canagaratna, M. R., Donahue, N. M., Prevot, A. S. H., Zhang, Q., Kroll, J. H., DeCarlo, P. F., Allan, J. D., Coe, H., Ng, N. L., Aiken, A. C., Docherty, K. S., Ulbrich, I. M.,
30 Grieshop, a P., Robinson, A. L., Duplissy, J., Smith, J. D., Wilson, K. R., Lanz, V. A., Hueglin, C., Sun, Y. L., Tian, J., Laaksonen, A., Raatikainen, T., Rautiainen, J., Vaattovaara, P., Ehn, M., Kulmala, M., Tomlinson, J. M., Collins, D. R., Cubison, M. J., Dunlea, E. J., Huffman, J. A., Onasch, T. B., Alfarra, M. R., Williams, P. I., Bower, K., Kondo, Y., Schneider, J., Drewnick, F., Borrmann,

- S., Weimer, S., Demerjian, K., Salcedo, D., Cottrell, L., Griffin, R., Takami, A., Miyoshi, T., Hatakeyama, S., Shimono, A., Sun, J. Y., Zhang, Y. M., Dzepina, K., Kimmel, J. R., Sueper, D., Jayne, J. T., Herndon, S. C., Trimborn, A. M., Williams, L. R., Wood, E. C., Middlebrook, A. M., Kolb, C. E., Baltensperger, U. and Worsnop, D. R.: Evolution of organic aerosols in the atmosphere., *Science* (80-.), 326(5959), 1525–1529, doi:10.1126/science.1180353, 2009.
- 5 Kampf, C. J., Jakob, R. and Hoffmann, T.: Identification and characterization of aging products in the glyoxal/ammonium sulfate system – Implications for light-absorbing material in atmospheric aerosols, *Atmos. Chem. Phys.*, 12(14), 6323–6333, doi:10.5194/acp-12-6323-2012, 2012.
- 10 Kourtchev, I., Fuller, S. J., Giorio, C., Healy, R. M., Wilson, E., O'Connor, I., Wenger, J. C., McLeod, M., Aalto, J., Ruuskanen, T. M., Maenhaut, W., Jones, R., Venables, D. S., Sodeau, J. R., Kulmala, M. and Kalberer, M.: Molecular composition of biogenic secondary organic aerosols using ultrahigh-resolution mass spectrometry: comparing laboratory and field studies, *Atmos. Chem. Phys.*, 14(4), 2155–2167, doi:10.5194/acp-14-2155-2014, 2014.
- 15 Kristensen, K., Enggrob, K. L., King, S. M., Worton, D. R., Platt, S. M., Mortensen, R., Rosenoern, T., Surratt, J. D., Bilde, M., Goldstein, A. H. and Glasius, M.: Formation and occurrence of dimer esters of pinene oxidation products in atmospheric aerosols, *Atmos. Chem. Phys.*, 13(7), 3763–3776, doi:10.5194/acp-13-3763-2013, 2013.
- 20 Kroll, J. H. and Seinfeld, J. H.: Chemistry of secondary organic aerosol: Formation and evolution of low-volatility organics in the atmosphere, *Atmos. Environ.*, 42(16), 3593–3624, doi:10.1016/j.atmosenv.2008.01.003, 2008.
- Kroll, J. H., Donahue, N. M., Jimenez, J. L., Kessler, S. H., Canagaratna, M. R., Wilson, K. R., Altieri, K. E., Mazzoleni, L. R., Wozniak, A. S., Bluhm, H., Mysak, E. R., Smith, J. D., Kolb, C. E. and Worsnop, D. R.: Carbon oxidation state as a metric for describing the chemistry of atmospheric organic aerosol., *Nat. Chem.*, 3(2), 133–9, doi:10.1038/nchem.948, 2011.
- 25 Krueve, A., Kaupmees, K., Liigand, J. and Leito, I.: Negative Electrospray Ionization via Deprotonation: Predicting the Ionization Efficiency, 2014.
- Law, W. S., Chen, H. W., Balabin, R., Berchtold, C., Meier, L. and Zenobi, R.: Rapid fingerprinting and classification of extra virgin olive oil by microjet sampling and extractive electrospray ionization mass spectrometry, *Analyst*, 135(4), 773–8, doi:10.1039/b924156f, 2010.
- 30 Lee, A., Goldstein, A. H., Keywood, M. D., Gao, S., Varutbangkul, V., Bahreini, R., Ng, N. L., Flagan, R. C. and Seinfeld, J. H.: Gas-phase products and secondary aerosol yields from the ozonolysis of ten different terpenes, *J. Geophys. Res.*, 111(D7), D07302,

doi:10.1029/2005JD006437, 2006.

Lignell, H., Epstein, S. A., Marvin, M. R., Shemesh, D., Gerber, B. and Nizkorodov, S.: Experimental and Theoretical Study of Aqueous cis -Pinonic Acid Photolysis, *J. Phys. Chem. A*, 117, 12930–12945, 2013.

- 5 Lindinger, W., Hansel, A. and Jordan, A.: Proton-transfer-reaction mass spectrometry (PTR-MS): On-line monitoring of volatile organic compounds at pptv levels, *Chem. Soc. Rev.*, 27(5), 347–354, 1998.

McCullough, B. J., Bristow, T., O'Connor, G. and Hopley, C.: On-line reaction monitoring by extractive electrospray ionisation, *Rapid Commun. Mass Spectrom.*, 25(10), 1445–51, doi:10.1002/rcm.5016, 2011.

- 10

Müller, L., Reinnig, M.-C., Naumann, K. H., Saathoff, H., Mentel, T. F., Donahue, N. M. and Hoffmann, T.: Formation of 3-methyl-1,2,3-butanetricarboxylic acid via gas phase oxidation of pinonic acid – a mass spectrometric study of SOA aging, *Atmos. Chem. Phys.*, 12(3), 1483–1496, doi:10.5194/acp-12-1483-2012, 2012.

- 15 Nah, T., Chan, M., Leone, S. R. and Wilson, K. R.: Real Time in Situ Chemical Characterization of Submicrometer Organic Particles Using Direct Analysis in Real Time-Mass Spectrometry, *Anal. Chem.*, 85, 2087–95, doi:10.1021/ac302560c, 2013.

Noziere, B., Kalberer, M., Claeys, M., Allan, J., Anna, B. D., Decesari, S., Finessi, E., Glasius, M., Grgic, I., Hamilton, J. F., Ho, T., Iinuma, Y., Jaoui, M., Kahnt, A., Kampf, C. J., Kourtchev, I., Maenhaut, W., Marsden, N., Saarikoski, S., Schnelle-kreis, J., Surratt, J. D., Szidat, S., Szmigielski, R. and Wisthaler, A.: The Molecular Identification of Organic Compounds in the Atmosphere: State of the Art and Challenges, *Chem. Rev.*, 115(10), 3919–3983, doi:10.1021/cr5003485, 2015.

- 20

Pankow, J. F.: An absorption model of the gas/aerosol partitioning involved in the formation of secondary organic aerosol, *Atmos. Environ.*, 28(2), 189–193, 1994.

- 25 Paulsen, D., Dommen, J., Kalberer, M., Prévôt, A. S. H., Richter, R., Sax, M., Steinbacher, M., Weingartner, E. and Baltensperger, U.: Secondary organic aerosol formation by irradiation of 1,3,5-trimethylbenzene-NO_x-H₂O in a new reaction chamber for atmospheric chemistry and physics., *Environ. Sci. Technol.*, 39(8), 2668–2678, doi:10.1021/es0489137, 2005.

Pereira, K. L., Hamilton, J. F., Rickard, A. R., Bloss, W. J., Alam, M. S., Camredon, M., Muñoz, A., Vázquez, M., Borrás, E. and Ródenas, M.: Secondary organic aerosol formation and composition from the photo-oxidation of methyl chavicol (estragole), *Atmos. Chem. Phys.*, 14(11), 5349–5368, doi:10.5194/acp-14-5349-2014, 2014.

- 30

Reinhardt, A., Emmenegger, C., Gerrits, B., Panse, C., Dommen, J., Baltensperger, U., Zenobi, R.

- and Kalberer, M.: Ultrahigh Mass Resolution and Accurate Mass Measurements as a Tool To Characterize Oligomers in Secondary Organic Aerosols, *Anal. Chem.*, 79(11), 4074–4082, doi:10.1029/2003GL018962.(16), 2007.
- 5 Saunders, S. M., Jenkin, M. E., Derwent, R. G. and Pilling, M. J.: Protocol for the development of the Master Chemical Mechanism, MCM v3 (Part A): tropospheric degradation of non-aromatic volatile organic compounds, *Atmos. Chem. Phys.*, 3, 161–180, 2003.
- Shilling, J. E., Chen, Q., King, S. M., Rosenoern, T., Kroll, J. H., Worsnop, D. R., DeCarlo, P. F., Aiken, a. C., Sueper, D., Jimenez, J. L. and Martin, S. T.: Loading-dependent elemental composition of α -pinene SOA particles, *Atmos. Chem. Phys.*, 9, 771–782, doi:10.5194/acp-9-771-2009, 2009.
- 10 Shiraiwa, M., Pfrang, C. and Pöschl, U.: Kinetic multi-layer model of aerosol surface and bulk chemistry (KM-SUB): the influence of interfacial transport and bulk diffusion on the oxidation of oleic acid, *Atmos. Chem. Phys.*, 10(1), 281–326, doi:DOI 10.5194/acp-10-3673-2010, 2010.
- Smith, D. and Spanel, P.: SELECTED ION FLOW TUBE MASS SPECTROMETRY (SIFT-MS) FOR ON-LINE TRACE GAS ANALYSIS, *Mass Spectrom. Rev.*, 661–700, doi:10.1002/mas.20033, 2005.
- 15 Turpin, B. J., Saxena, P. and Andrews, E.: Measuring and simulating particulate organics in the atmosphere: problems and prospects, *Atmos. Environ.*, 34(18), 2983–3013, doi:10.1016/S1352-2310(99)00501-4, 2000.
- Vogel, A. L., Äijälä, M., Corrigan, A. L., Junninen, H., Ehn, M., Petäjä, T., Worsnop, D. R., 20 Kulmala, M., Russell, L. M., Williams, J. and Hoffmann, T.: In situ submicron organic aerosol characterization at a boreal forest research station during HUMPPA-COPEC 2010 using soft and hard ionization mass spectrometry, *Atmos. Chem. Phys.*, 13(21), 10933–10950, doi:10.5194/acp-13-10933-2013, 2013.
- Wisthaler, A., Jensen, N. R., Winterhalter, R., Lindinger, W. and Hjorth, J.: Measurements of 25 acetone and other gas phase product yields from the OH-initiated oxidation of terpenes by proton-transfer-reaction mass spectrometry (PTR-MS), *Atmos. Environ.*, 35(February), 6181–6191, 2001.
- Wu, C., Siems, W. F. and Hill Jr., H. H.: Secondary Electrospray Ionization Ion Mobility Spectrometry / Mass Spectrometry of Illicit Drugs, *Anal. Chem.*, 72(2), 396–403, 2000.
- Yatawelli, R. L. N., Stark, H., Thompson, S. L., Kimmel, J. R., Cubison, M. J., Day, D. A., 30 Campuzano-Jost, P., Palm, B. B., Hodzic, A., Thornton, J. A., Jayne, J. T., Worsnop, D. R. and Jimenez, J. L.: Semicontinuous measurements of gas–particle partitioning of organic acids in a ponderosa pine forest using a MOVI-HRToF-CIMS, *Atmos. Chem. Phys.*, 14(3), 1527–1546, doi:10.5194/acp-14-1527-2014, 2014.

- Zhang, X., McVay, R. C., Huang, D. D., Dalleska, N. F., Aumont, B., Flagan, R. C. and Seinfeld, J. H.: Formation and evolution of molecular products in α -pinene secondary organic aerosol., *Proc. Natl. Acad. Sci. U. S. A.*, 112(46), 14168–73, doi:10.1073/pnas.1517742112, 2015.
- Zhao, Y., Chan, J. K., Lopez-Hilfiker, F. D., McKeown, M. A., Ambro, E. L. D., Slowik, J. G.,
5 Riffell, J. A. and Thornton, J. A.: An electrospray chemical ionization source for real-time measurement of atmospheric organic and inorganic vapors, *Atmos. Meas. Tech.*, 3609–3625, 2017a.
- Zhao, Y., Fairhurst, M. C., Wingen, L. M., Perraud, V. and Ezell, M. J.: New insights into atmospherically relevant reaction systems using direct analysis in real-time mass spectrometry (DART-MS), , 1373–1386, doi:10.5194/amt-10-1373-2017, 2017b.
- 10 Zhu, L., Hu, Z., Gamez, G., Law, W. S., Chen, H., Yang, S., Chingin, K., Balabin, R. M., Wang, R., Zhang, T. and Zenobi, R.: Simultaneous sampling of volatile and non-volatile analytes in beer for fast fingerprinting by extractive electrospray ionization mass spectrometry, *Anal. Bioanal. Chem.*, 398(1), 405–13, doi:10.1007/s00216-010-3945-8, 2010.
- Zielinski, A. ., Kourtchev, I. ., Bortolini, C. ., Fuller, S. J. ., Giorio, C. ., Popoola, O. ., Bogialli, S.
15 ., Tapparo, A. ., Jones, R. L. . and Kalberer, M.: A new processing scheme for ultra-high resolution direct infusion mass spectrometry data, *Talanta*, submitted, 2017.
- Ziemann, P. J. and Atkinson, R.: Kinetics, products, and mechanisms of secondary organic aerosol formation, *Chem. Soc. Rev.*, 41(19), 6582–605, doi:10.1039/c2cs35122f, 2012.

Supporting Information for **“Online molecular characterisation of organic aerosols in an atmospheric chamber using Extractive Electrospray Ionisation Mass Spectrometry”** by P.J. Gallimore et al.

5

Experimental setup

The experimental apparatus used for production and classification of standard aerosols (section 2.1) and for the simulation chamber experiments (section 2.2) are shown below.

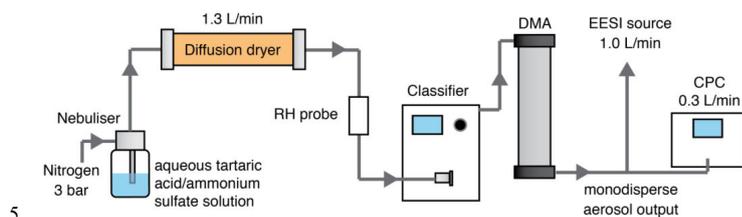


Figure S1: Aerosol flow setup used for producing, classifying and measuring the chemical composition of model aerosols to quantify the extraction process.

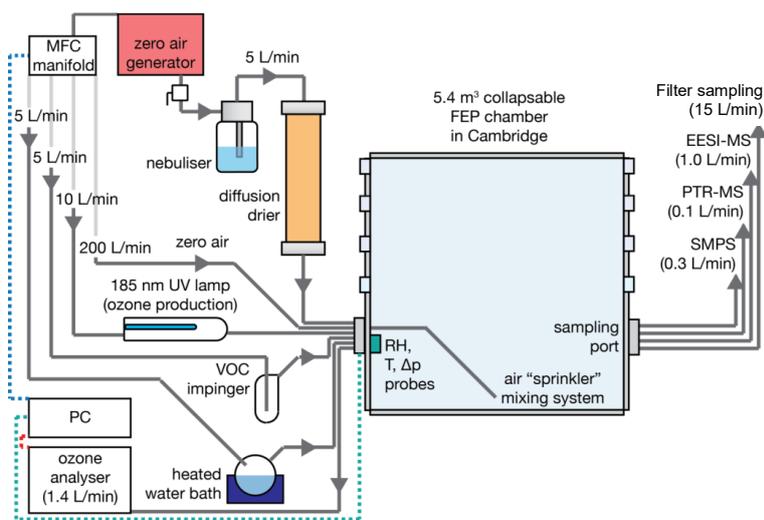


Figure S2: Operational details for the Cambridge Atmospheric Simulation Chamber (CASC), adapted from Gallimore et al., (2017b). The 5.4 m³ chamber enables study of secondary organic aerosol formation and aging processes in the laboratory; water vapour, seed aerosols, atmospheric oxidants and volatile organic compounds can be introduced under controlled conditions. A variety of instrumentation is attached to characterise the resulting chemistry, including a recently-developed extractive electrospray ionisation mass spectrometer (EESI-MS) to detect organic aerosol components.

Flow conditions in the EESI batch sampling system

This section considers the flow and mixing characteristics in the 10 L sampling reservoir (dimensions $\sim 92 \times 12$ cm) described in section 2.3. The 1 L min^{-1} “pushing flow” was introduced under laminar flow conditions (Reynolds number ~ 12). The total introduction of air was 3.5 L over
5 3.5 minutes, corresponding to a nominal distance of 32 cm along the flow tube. The extent of additional mixing beyond this volume displacement will be determined by molecular diffusion, described by Equation S1:

$$\tau = \frac{l^2}{D} \quad (\text{S1})$$

10 Where τ is the diffusion time, l is the diffusion length and D is the diffusion coefficient of air. Diffusion of accumulation mode particles will be negligible by comparison. For an introduction time of 3.5 minutes and diffusion coefficient $0.2 \text{ cm}^2 \text{ s}^{-1}$, the diffusion length is 6.5 cm. Therefore only the first $\sim 40\%$ of the tube length, furthest from the MS sampling, will be influenced by zero air
introduction.

15

The EESI-MS signal is also relatively consistent across each 3.5 minute sampling period (Figure 3), confirming that this cycling does not significantly affect the sampled particle composition.

Reaction scheme for MCM simulations

The reaction scheme for the degradation of α -pinene is based on the mechanism described in Saunders et al., (Saunders et al., 2003). All reactions involving the ozone-initiated oxidation of α -pinene and its products, including decomposition of reaction intermediates and secondary OH-mediated chemistry, were extracted from the MCM website (<http://mcm.leeds.ac.uk/MCM>) in June 2017. This mechanism extract comprises 313 explicit species.

We also included an auxiliary reaction to approximate the gradual introduction of ozone into the chamber (reaction S2):



Pre-O₃ does not participate in any other reactions, and is converted into O₃ on a timescale $\tau_{\text{pre}} = 1/k_{\text{pre}} = 3\text{-}30$ minutes, adjusted to reflect the experimental timescale for ozone introduction for each experiment.

The simulations were initialised with all species concentrations set to zero, apart from: α -pinene (APINENE), which was set to 45, 100 and 500 ppb for the low, medium and high concentration experiments respectively, and pre-O₃ (PREO3) which was adjusted to simulate the observed [O₃]_{max} in each experiment (Table 1).

Formatted: Font: Bold

Formatted: Font: 10 pt

Formatted: Subscript

Formatted: Subscript

Formatted: Font: 10 pt

Formatted: Font: 10 pt

Formatted Table

Formatted: Right

Formatted: Subscript

Formatted: Subscript

Formatted: Font: Italic

Formatted: Subscript

Formatted: Font: Italic

Formatted: Subscript

Formatted: Subscript

Formatted: Subscript

Formatted: Subscript

Extraction efficiency of tartaric acid in mixed organic-inorganic aerosols


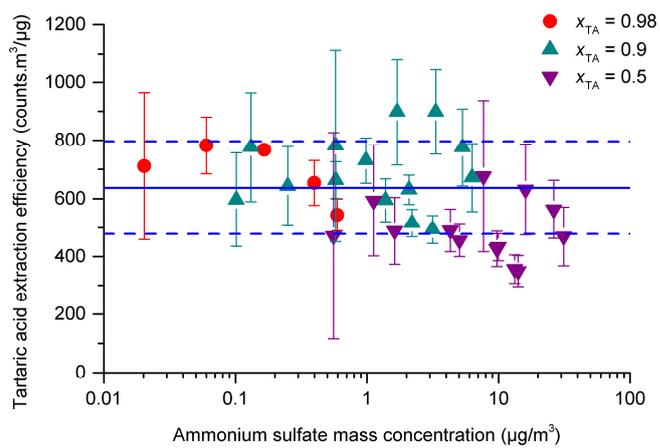


Figure S3: Tartaric acid MS signal, normalised by the tartaric acid aerosol mass, as a function of the ammonium sulfate aerosol mass. The blue solid and dotted lines represent the mean and standard deviation respectively of measurements on single-component tartaric acid aerosols ($x_{TA} = 1$).

5


Mass spectra for EESI-MS and PTR-MS

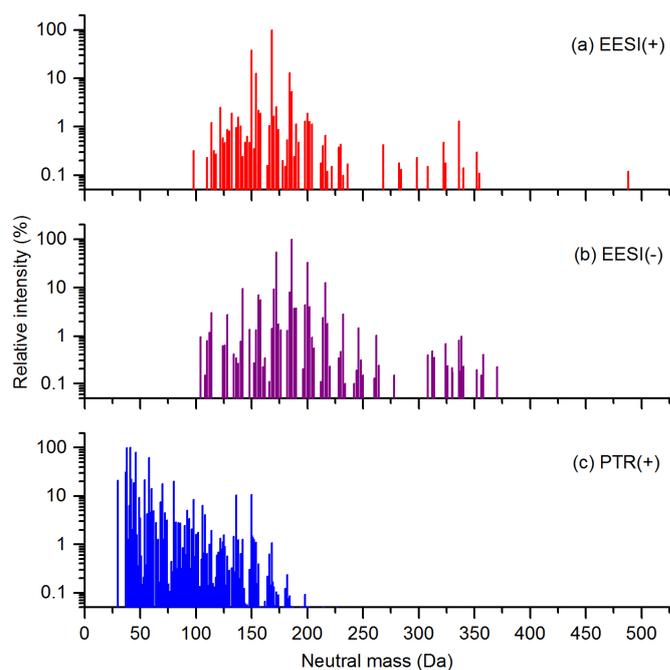

5 Figure S4: Mass spectra obtained during the dark ozonolysis of α -pinene under “medium” conditions (Table 1) using three online MS techniques: (a) EESI-MS in positive ionisation mode, (b) EESI-MS in negative ionisation mode and (c) PTR-MS using H_3O^+ as a chemical ionisation reagent. The ions have been assigned to molecular formulae and are plotted as neutral masses to aid comparison. Only PTR-MS ions corresponding to assigned α -pinene ozonolysis products are shown. Taken together, the three techniques enable online detection of a wide variety of organic compound classes and volatilities, from hydrocarbons such as α -pinene to highly oxidised carboxylic acids.


10

Comparison between EESI(-) and nanoESI(-) spectra

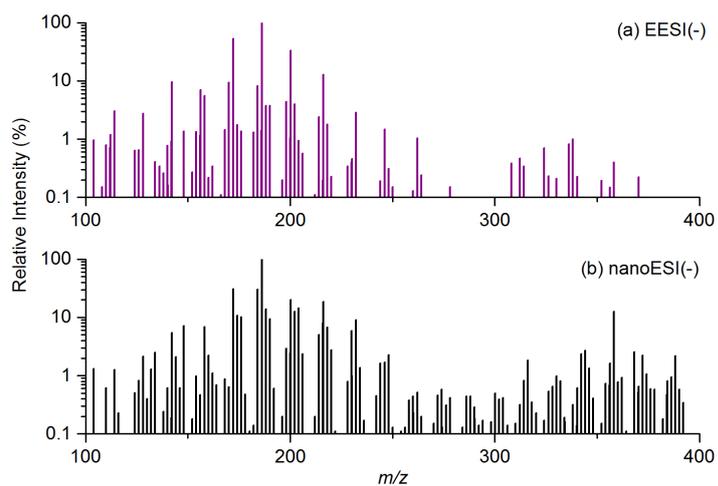



5 **Figure S5: Mass spectra obtained during the dark ozonolysis of α -pinene under “medium” conditions (Table 1) using (a) online EESI-MS in negative ionisation mode and (b) nanoESI-MS of SOA filter extracts. The online MS was acquired and the filter collected 1 hour after the start of ozonolysis in the chamber. The spectra are very similar in the monomer region (<250 Da), but the oligomers detected are more numerous and possess slightly higher molecular weights in the nanoESI(-) spectrum.**

Comparison between measured MS intensities and MCM concentrations for oxidation products

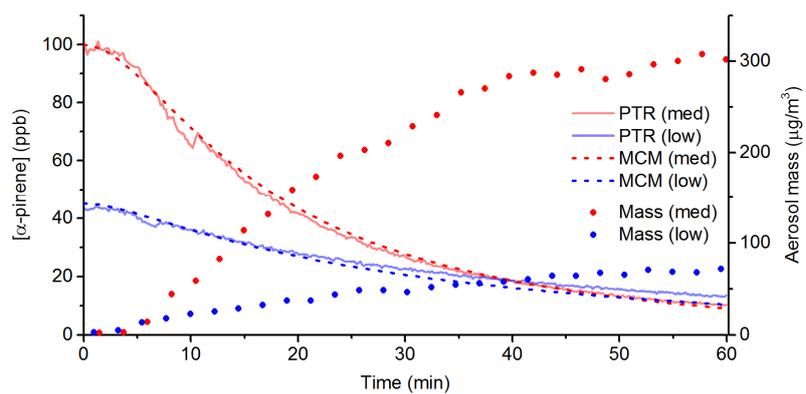


5 **Figure S56:** α -pinene loss and SOA production during chamber experiments with varying $[\alpha\text{-pinene}]_0$, showing only the medium and low concentration conditions. Dashed lines: measured $[\alpha\text{-pinene}]$ from PTR-MS; Solid lines: MCM simulated $[\alpha\text{-pinene}]$; Points: measured aerosol mass from SMPS.

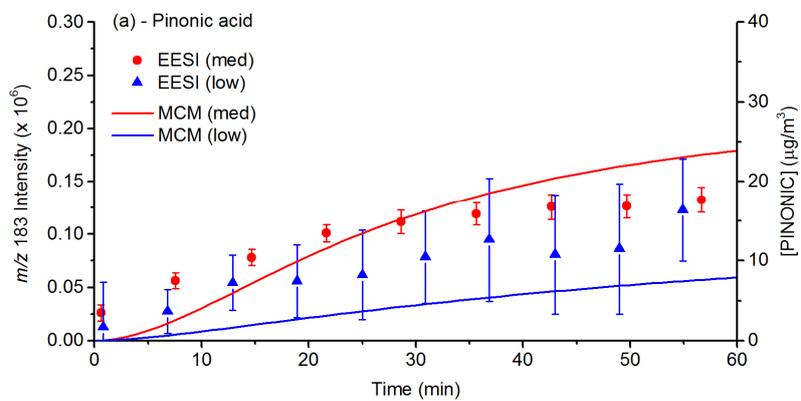

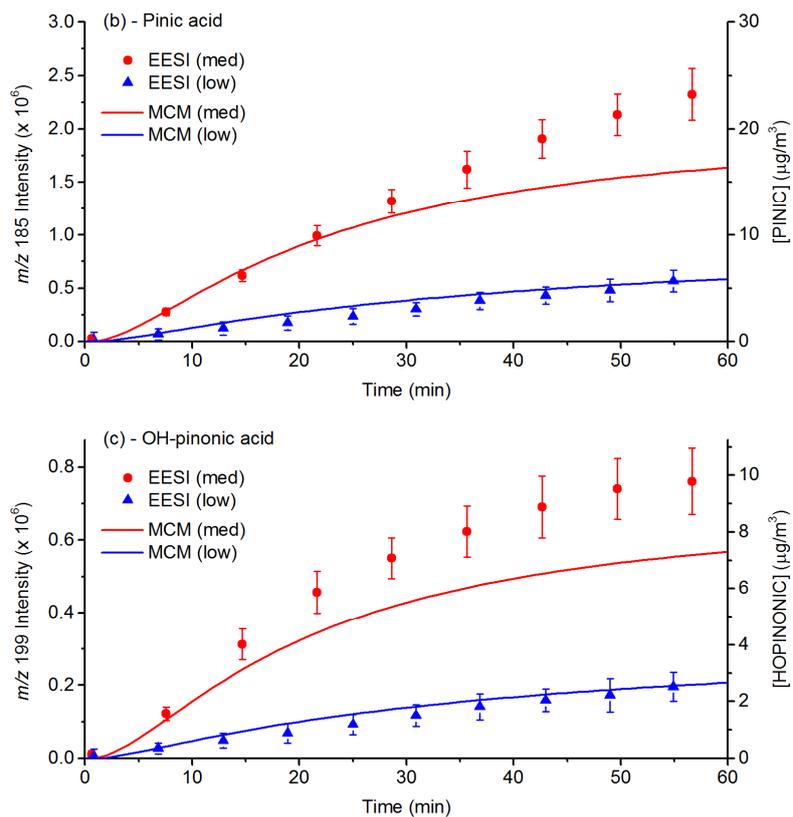

5 | **Figure S67:** Comparison between EESI-MS intensities (left y-axis) and MCM simulated concentrations (right y-axis) for (a) pinonic acid, (b) pinic acid and (c) OH-pinonic acid, showing only the medium and low concentration conditions. The scales of the y-axes from Figure 87 have been divided by 4, so that the relative scaling between the m/z and MCM axes is consistent with Figure 87.

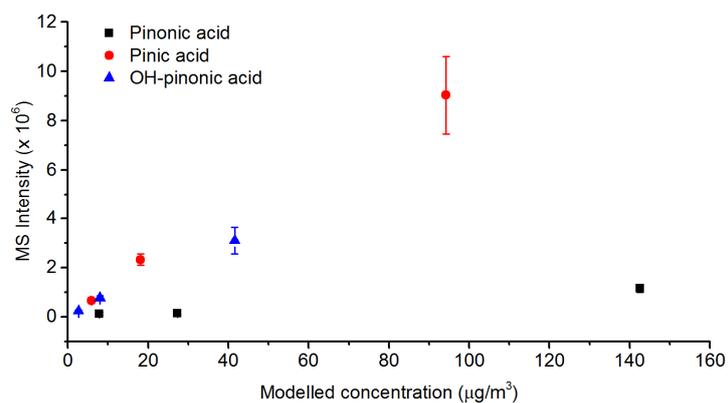

5 **Figure S78:** MS intensity of pinonic, pinic and OH-pinonic acids as a function of predicted MCM concentrations. The data shown are for the measurements approximately 1 hour after the start of ozonolysis in Figure S7, where the rate of change of concentration slows and hence simulated and measured concentrations represent approximate final yields.

References

10 Saunders, S. M., Jenkin, M. E., Derwent, R. G. and Pilling, M. J.: Protocol for the development of the Master Chemical Mechanism, MCM v3 (Part A): tropospheric degradation of non-aromatic volatile organic compounds, Atmos. Chem. Phys., 3, 161–180, 2003.

Formatted: Normal

Formatted: Font: Bold

Formatted: Normal